



| | |
|---|-------|
| SGE GC Capillary Column innovation, manufacture and selection | 74-82 |
| 100% Dimethyl Polysiloxane | |
| BP1 | 83 |
| BP1 PONA | 84 |
| BPX1 | 84 |

GC Capillary Columns

| | |
|---|--------|
| 100% Dimethyl Polysiloxane in a Sol-Gel Matrix SolGel-1ms™ | 85 |
| 5% Phenyl / 95% Dimethyl Polysiloxane BP5 | 86 |
| 5% Phenyl Polysilphenylene-siloxane BPX5 | 87-88 |
| 5% Phenyl Polycarborane-siloxane HT5 | 89 |
| 8% Phenyl Polycarborane-siloxane HT8 | 90 |
| 35% Phenyl Polysilphenylene-siloxane BPX35 | 90-91 |
| 35% Phenyl Polysilphenylene-siloxane BPX608 | 91 |
| 50% Phenyl Polysilphenylene-siloxane BPX50 | 92 |
| 70% Cyanopropyl Polysilphenylene-siloxane BPX70 | 92-93 |
| 90% Cyanopropyl Polysilphenylene-siloxane BPX90 | 93 |
| Polyethylene Glycol (PEG) in a Sol-Gel matrix SolGel-WAX™ | 94 |
| Polyethylene Glycol BP20 (WAX) | 94-95 |
| Polyethylene Glycol (PEG) – TPA Treated BP21 (FFAP) | 95-96 |
| 14% Cyanopropylphenyl Polysiloxane BP10 (1701) | 96 |
| 50% Cyanopropylphenyl Polysiloxane BP225 | 97 |
| Cyanopropylphenyl Polysiloxane BPX-VOLATILES | 97 |
| Cyanopropylphenyl Polysiloxane BP624 | 98 |
| Permethyated Beta-Cyclodextrin (Chiral) CYDEX-B™ | 98 |
| GC Applications by Industry | 99-146 |

SGE's silica drawing towers where continuous lengths of fused silica are drawn and coated.

- Five decades of capillary column innovation.
- End to end capillary column manufacture.
- Providing separation solutions.



Five Decades of Capillary Column Innovation



SGE has a long history developing and producing GC capillary columns, with SGE's founder Ernest Dawes first being involved making glass capillary columns in 1959.

That expertise has been built upon with the development of leading capabilities in glass technology, polymer synthesis, surface chemistry and production processes all combined with an intimate knowledge of chromatography.

SGE develops and synthesizes specialty polymers leading to SGE being the first, and often only, capillary chromatography company to offer many types of GC stationary phases. SGE was the first to introduce the now industry standard silarylene phases in 1987 with their improved thermal stability, as well as SolGel in 1999 and the carborane phases in 1987. A detailed explanation of how these polymers work can be found on pages 76-80.

End to End Capillary Column Manufacture

SGE has long been a manufacturer of GC capillary columns with the complete technology capability to produce the finest capillary columns from beginning to end, including the special requirements of producing the fused silica capillary tubing. This end to end manufacturing capability allows SGE to control the fabrication process precisely to produce the finest quality capillary columns available.

The individual technologies SGE employs in GC capillary column manufacture are:

- Drawing of the precision fused silica capillary tubing.

- Developing and synthesizing the specialty polymer stationary phases.
- Performing the specialty chemical treatment of the fused silica surface so that it is inert and compatible for the cross-linked stationary phase.
- Coating and cross-linking the polymer stationary phase.
- Quality testing of every completed capillary column to rigorous standards.



[Click to Play Video](#)

Fused Silica

The process of producing fused silica at SGE is carried out on a series of sophisticated drawing towers with fine control of conditions and feedback loops to automatically make adjustments to the conditions. This ensures superb dimensional control and strength which is verified through stress proof testing of all material. By producing the fused silica ourselves, SGE has complete control of this important aspect of producing the highest quality GC capillary columns.

The fused silica used by SGE is very high purity devoid of impurities such as metal oxides found in conventional glasses. Depending on the application, SGE offers two types of FST coating - polyimide (max temp 400 °C) and aluminum (max. temperature 480 °C). SGE's capillary columns operate comfortably to 400 °C (dependent on the phase selected).

Stationary Phase Polymer

SGE has designed its phase synthesis so that most capillary columns may be washed with solvent to remove any contamination. When a capillary column's performance has deteriorated from extended use or contamination, performance can often be restored though washing with a suitable solvent. See page 196 for details and equipment available for washing capillary columns.

Rigorous Performance Testing

Test criteria are selected based on the applications that different capillary column types are targeted for, to ensure the capillary column meets the standards for that analysis. General purpose capillary columns are tested to ensure they meet inertness standards for difficult to chromatograph compounds, and run at conditions and levels designed to highlight variations in capillary column performance. For example, SGE's non-polar phase BPX5 is tested using active probes

such as n-decylamine and 2,4-dinitrophenol chromatographed at low concentrations (1-2 nanogram on capillary column for 0.25 µm film thickness) and with sufficient retained time on the run to induce tailing on all but the most highly inert capillary column. SGE does not offer separate ranges of capillary columns of different performance levels – all SGE GC capillary columns meet these high standards.

Retention Time and Consistency

Because SGE controls the capillary column fabrication process from beginning to end we are also able to achieve remarkably consistent retention characteristics from column to column. When a method is established on an SGE column, the same separation can be expected column after column.

Thermal Stability

A long term issue in capillary GC is the breakdown of the stationary phase in the capillary column at elevated temperatures which leads to rising and noisy baseline signals thereby limiting sensitivity of the analysis. Stationary phase breakdown at elevated temperatures cannot be eliminated but it can be reduced dramatically through improving the technology. SGE developed, and was the first to introduce, silarylene - containing polymers such as silphenylene stationary phases in 1987. Silphenylene phases replace some of the oxygen atoms in the backbone of the siloxane polymer with aromatic groups. This led to a dramatically improved thermal stability for GC phases with silphenylene phases now available in a wide range of polarities and selectivities. SGE capillary columns are monitored for bleed performance with rigorous standards established. Bleed is measured and specified in terms of detector signal and calibrated to "nanograms of siloxane per second" eluted from the capillary columns. **The test is performed at the maximum operating temperature for the capillary column.**



The measure for bleed of nanograms of siloxane per second eluting from the capillary column is more meaningful than exclusively reporting picoamp FID signal. Picoamp signal is highly dependent on the detector and conditions used and is not an

absolute measure. SGE carries out the bleed measurement on FID to assure the best performance possible.

Below is an example of the SGE GC Capillary Column Performance Report.


GC Columns and Applications

Part Number:
Re-order information.

Serial Number Column Traceability:
Every SGE GC column is traceable back to its manufacture.

Measure of Theoretical Plates/meter:
This is a measure of the efficiency of the column.

Maximum continuous temperature:
This is the maximum recommended temperature for the column. Higher temperatures can be used, but this will reduce column lifetime.

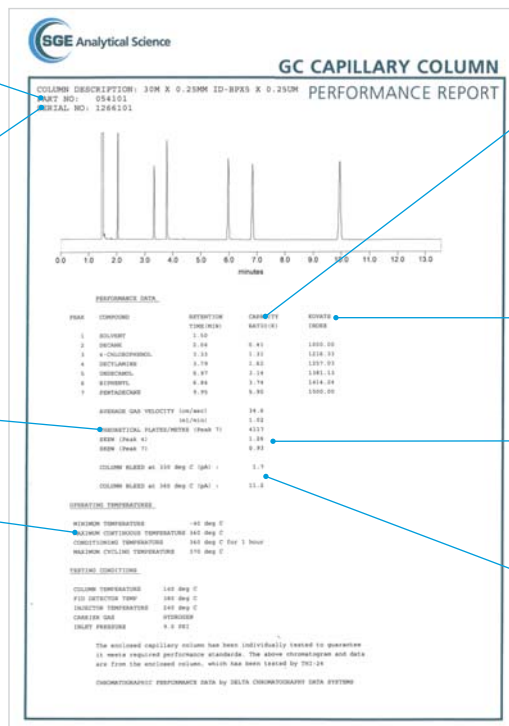

Capacity Ratio:
This is a measure of the film thickness.

Kovats Index:
Describes the retention behavior of a compound relative to that of straight chain hydrocarbons. Especially important for more polar columns.

Skew:
This is a measure of the degree of tailing (1.0 = Perfect).

Thermal Stability:
Each column is bleed tested to its maximum continuous operating temperature.

Providing Separation Solutions

GC Capillary Columns Polarity Scale

SGE strives to develop a better understanding of the interactions of the solute molecules with the GC stationary phase types in our product range and those we could design and synthesize. The objective is to be able to assist you the chromatographer to select a GC stationary phase for the separation of particular classes of compounds.

All chromatographers want the best separation and need to focus on the key parameters that influence the resolution equation. R can be viewed in three sections consisting of variables which influence capillary column efficiency, retention and selectivity.

$$R = \left(\frac{\sqrt{N}}{4} \right) \left(\frac{k}{k+1} \right) \left(\frac{\alpha-1}{\alpha} \right)$$

Column Efficiency
Retention
Selectivity

R = resolution, N = theoretical plates, k = capacity factor, α = selectivity

Another way of viewing the resolution equation from the GC capillary column perspective is that quality impacts the capillary column efficiency, the physical dimensions of the capillary column influence retention and the phase chemistry dictates selectivity. Inevitably, many GC operators focus on flow rates and temperatures because of their importance in getting good peak shapes and nice separations – rarely do we pay attention to how the phase can have such an effect on the relative retention time. The fine detail of the chromatography comes in the interaction with the phase.


Stationary Phase Polarity

A discussion on phase chemistry inevitably involves a reference to polarity – polarity in general terms and where phases fit along a linear polarity scale – but there is more

to it than this. There are different types of interactions based on the different types of functionality of the GC stationary phase polymer. In trying to create a scaled representation of the mechanisms of separation SGE has placed the stationary phases against a qualitative scale, although this scale is analyte dependent. The scale reflects the relative ability of phases to interact with particular types of analytes.

The scales shown in the 3D Phase Polarity diagram below, are qualitative rather than quantitative and have been derived from experimental work studying the retention of different analytes in the different types of stationary phases. Essentially the focus has been to develop a three dimensional representation of where each phase fits as a point on a plot of three classic bonding mechanisms - 'Van der Waals', H-bonding and π -bonding.

3D Phase Polarity Scale

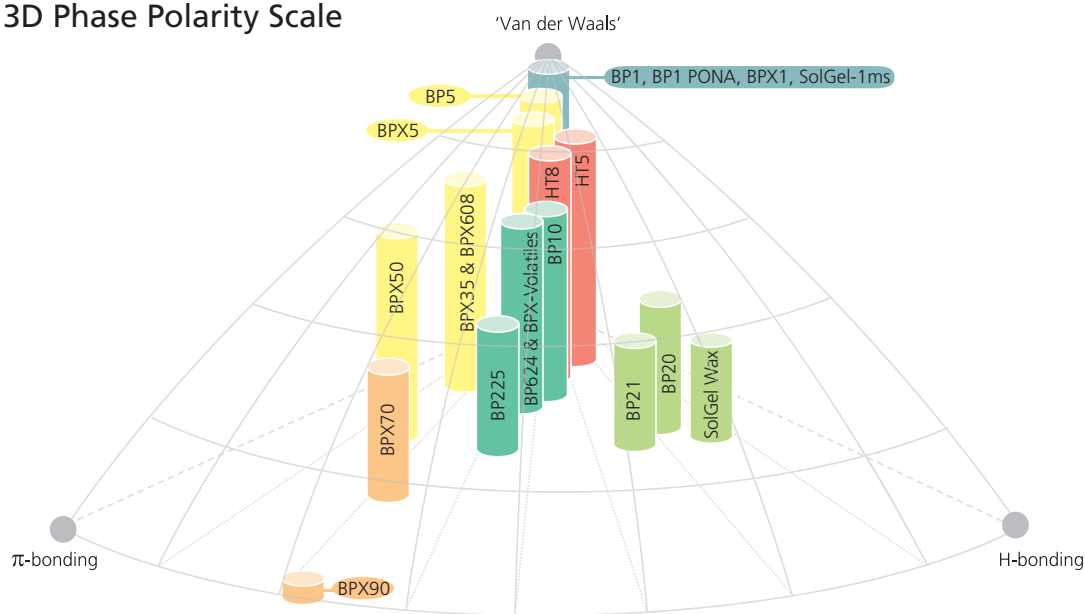

- Dimethyl Polysiloxane
- Phenyl Polysilphenylene Siloxane
- Cyanopropyl Polysilphenylene Siloxane
- Polycarborane Siloxane
- Polyethylene Glycol
- Cyanopropylphenyl Siloxane

Bonding Mechanisms

Van der Waals – essentially electrostatic attraction from temporary dipoles and are a very weak interaction. They are at their greatest relative contribution in the non-polar phases like the dimethylsiloxanes.

Hydrogen bonding results from the attraction of positive and negative charges of hydrogen and non-bonding pairs of electrons and is the force that holds water molecules together as liquid.


The π -bonding is associated with the aromatic class of compounds that include

benzene rings. Molecules with these loose clouds of donut shaped electronic charges have their own attraction towards each other. The π -bond in benzene is perpendicular to the benzene ring bonds so they interact more easily if the shape of the molecules does not create steric hindrance.

Stationary phases consist of basic polymer units with functionalities that can be modified by the addition of various moieties during synthesis. These moieties can be added in various amounts to create different concentrations of a particular functionality.



SGE GC Capillary Column Phases

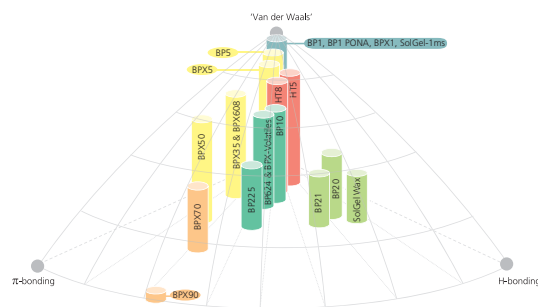


GC Columns and Applications

| Color Code | Phase | Structure | SGE Phase | Characteristics |
|------------|--|---|---|--|
| ● | Dimethyl Polysiloxane | $\left[\begin{array}{cc} \text{CH}_3 & \text{CH}_3 \\ & \\ \text{---Si---O---Si---O---} \\ & \\ \text{CH}_3 & \text{CH}_3 \end{array} \right]_n$ | BP1 BP1 PONA BPX1 SolGel-1ms | <ul style="list-style-type: none"> Polydimethylsiloxane (PDMS) "non-polar" type phases which rely on Van der Waals interactions between molecules and separate primarily based on "boiling point" type separation. Useful chromatographic space is usually considered in terms of modifications to non-polar retention. This is understandable because the GC is useful for volatile compounds and that usually means organics. Organics that can be vaporized are generally high in non-polar (alkane or hydrocarbon) character. It is this part of their surface that allows them to be soluble in a non-polar phase. It is also this characteristic that makes the BP1 (dimethylsiloxane) a universal phase. |
| ● | Diphenyl Dimethyl Siloxane (Phenyl substituted Siloxanes) | $\left[\begin{array}{cc} \text{C}_6\text{H}_5 & \text{C}_6\text{H}_5 \\ & \\ \text{---Si---O---Si---O---} \\ & \\ \text{CH}_3 & \text{CH}_3 \end{array} \right]_n$ | BP5 | <ul style="list-style-type: none"> The classical 5% phenyl group of phases |
| ● | Phenyl Polysilphenylene Siloxane (Silphenylene substituted Polydimethylsiloxane) | $\left[\begin{array}{cc} \text{C}_6\text{H}_5 & \text{C}_6\text{H}_5 \\ & \\ \text{---Si---O---Si---O---} \\ & \\ \text{C}_6\text{H}_4 & \text{C}_6\text{H}_4 \end{array} \right]_n$ | BPX5 BPX35 BPX608 BPX50 | <ul style="list-style-type: none"> Silphenylene phases have become fairly common now with many manufacturers offering at least some phases of this type, SGE has a full range. Phases with the "X" notation have a silphenylene backbone (exception is the BPX1). Phenyl substituted polymers are relatively non-polar and rely for their different functionality on π - bonding with the aromatic phenyl groups. SGE was the first GC capillary column manufacturer to introduce this type of phase commercially in the 1980s with the intention of improving the thermal stability to give higher maximum temperatures and reduced bleed. |
| ● | Polycarborane Siloxane | $\left[\begin{array}{c} \text{C}_6\text{H}_5 \\ \\ \text{---Si---O---} \\ \\ \text{C}_6\text{H}_5 \end{array} \right]_n$ | HT5 HT8 | <ul style="list-style-type: none"> The carborane phases were originally developed as very high thermal stability phases for high temperature work to 460 °C. The functionality of the carboranes is difficult to explain – they end up with pentavalent bonds with shared sigma bonds rather than π - bonds. The bonds are transient like a benzene with a ball of shared electrons. HT5 and HT8 are low π - bonding purely due to the low concentration of carborane in the polymer, otherwise it would be high. |
| ● | Cyanopropylphenyl Siloxane | $\left[\begin{array}{cc} \text{CH}_3 & \text{CN} \\ & \\ \text{---Si---O---Si---O---} \\ & \\ \text{CH}_3 & \text{C}_6\text{H}_5 \end{array} \right]_n$ | BP225 BP10 BP624 BPX-Volatiles | <ul style="list-style-type: none"> 'Polar' phases with <50% cyanopropyl substituted dimethylpolysiloxane. |
| ● | Cyanopropyl Polysilphenylene Siloxane | $\left[\begin{array}{cc} \text{C}_6\text{H}_5 & \text{CN} \\ & \\ \text{---Si---O---Si---O---} \\ & \\ \text{C}_6\text{H}_4 & \text{C}_6\text{H}_4 \end{array} \right]_n$ | BPX70 BPX90 | <ul style="list-style-type: none"> High cyanopropyl substituted phases, are more difficult to make as efficient, thermally stable phases. BPX70 is equivalent to and behaves like a 70% cyanopropyl siloxane but with siphenyl end substituted backbone for stability which was introduced in 1987 and remained the most polar thermally stable phase for a long time. BPX90 which is equivalent to a 90% cyanopropyl siloxane and stable to 300 °C which is excellent for such a polar phase. The prominent interaction for BPX90 is π - π bonding with the cyano group; the cyano groups become almost entirely responsible for the partitioning. |
| ● | Polyethylene Glycol | $\left[\text{CH}_2 - \text{CH}_2 - \text{O} \right]_n$ | BP21 BP20 SolGel-WAX™ | <ul style="list-style-type: none"> (PEG) 'wax' type phases where the main separation mechanisms are hydrogen bonding or dipole interactions. The wax phases are often considered as ideal for mixtures of chemically different components such as those contained in essential oils. |

Choosing the Right Phase for Your Separation


So how can you use this elaborate explanation of phases and bonding types? The answer is simple! In separation science we seek solutions in resolving complex mixtures and a "one-phase fits all" is more a hope than a reality. Here SGE has explored different phases from a polarity scale to assist the chromatographer to choose the best combination of phases which provide an orthogonal solution rather than a simple variation of a theme.

Take for example the separation of aromatics on the polyethylene glycol capillary column BP20 (H-bonding) compared to BP1 where the primary interaction is Van der Waals. Whereas para- and meta-xylene are unresolved on BP1, they are clearly resolved on BP20 with a corresponding change in elution order to the alkanes. This is an interesting interaction because the aromatic xylenes have been attracted by the H-bond rich BP20. It is not a totally 'one or the other' situation when judging the contribution of H-bond and π -bond affinities, because they have some affinity for each other.

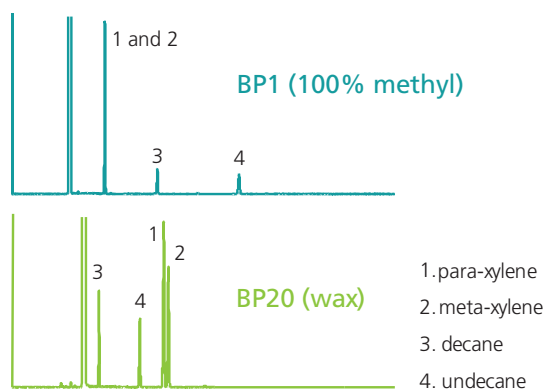

A higher component separation is demonstrated with a series of hydrocarbons run on a relatively non-polar phase (BPX5, on the x-axis in figure above right) and on a highly polar BPX90 with the retention times plotted on the y-axis. If the hydrocarbon family is split up on the basis of unsaturated

groups, this extra dimension shown in color (chemical group) reveals that the plot shows strong correlations for retention characteristics and functional chemistry.

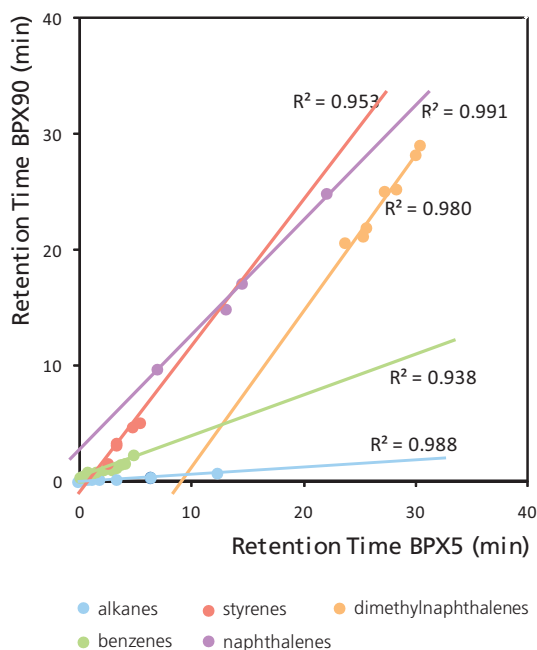

In this case, the hydrocarbon alkanes (light blue) are completely non-polar. They are retained on the phase only because the phase has sufficient non-polar character to interact with them. In the case of BPX90, it is so polar that it does not offer alkanes the opportunity for interaction. As a result, the alkanes tend to elute almost unretained. The alkanes show almost perfect orthogonality here. Retention on BPX5 versus no retention on BPX90 – they lie almost along the x-axis. We can now reason that if pure hydrocarbons (Van der Waals or non-polar interactions) give little or no BPX90 retention then retention of the remaining aromatics is due to purely π type interactions. When comparing GC phases, departures from the diagonal mark a significant change in the retention mechanism.

In conclusion, polar phases offer selectivity based on functionality rather than on Van der Waals interactions and are an ideal choice for the separation of analytes that were unresolved on non-polar or moderately polar phases.

GC Columns and Applications



The primary advantages of considering phase selectivity include:


- 2D GC – the choice of orthogonal chemistries for the 1st and 2nd dimensions.
- Fast GC – highly retained analytes on non-polar phases elute much earlier on polar phases.
- Ubiquitous FAMES methods.
- Separation of unresolved analytes due to alternative functionality.

SGE hopes this information assists in your understanding of optimum GC capillary column phase selection for your application. Following is a summary of phase, plus other capillary column parameters such as internal diameter, capillary column length and film thickness, to assist with identification of the right SGE GC capillary column for your separation solution.



GC Capillary Column Selection

1. Stationary Phase

- Select the least polar phase that will perform the separation you require.
- Non-polar stationary phases separate analytes predominantly by order of boiling point. Increase the amount of phenyl and/or cyanopropyl content in the phase, and the separation is then influenced more by differences in dipole moments or charge distributions (BP10 (1701), BPX35, BPX50, BP225 and BPX70).

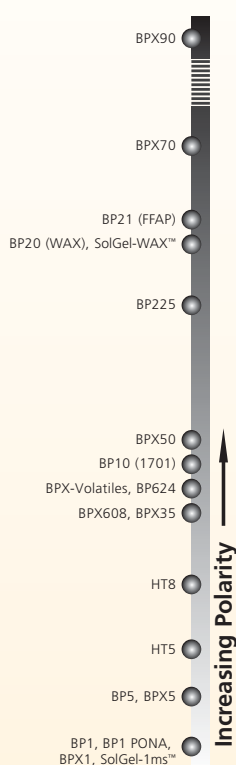

OPs on Aromatic Phases

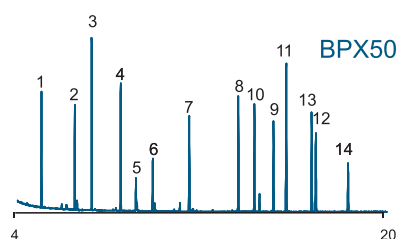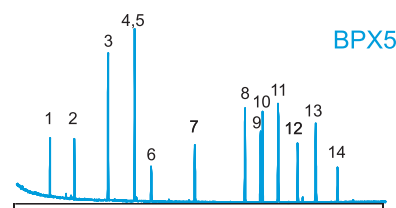

Organophosphorus Pesticides

- | | |
|-------------------------------------|------------------------|
| 1. 4-Chloro-3-nitrobenzotrifluoride | 7. Chlorfenvinphos |
| 2. 1-Bromo-2-nitrobenzene | 8. Ethion |
| 3. Tributylphosphate | 9. Famphur |
| 4. Terbufos | 10. Carbophenothion |
| 5. Dioxathion | 11. Triphenylphosphate |
| 6. Phoshamidon | 12. Phosmet |
| | 13. Leptophos |
| | 14. Azinphos-ethyl |


| | |
|----------------|-------------------------------|
| Columns | 30 m x 0.25 mm x 0.25 µm |
| Initial Temp | 45 °C (1 min) |
| 1st Temp Ramp | 30 °C/min to 200 °C (0.1 min) |
| 2nd Temp Ramp | 7 °C/min |
| Final Temp | 315 °C (hold 10 min) |
| Injector Temp | 280 °C |
| Splitless Time | 1 min |
| Carrier | He, 1 ml.min |
| Instrument | HP 6890/5973 |

Effect of increasing Phenyl content in the stationary phase.

- To separate compounds that differ more in their hydrogen bonding capacities (for example aldehydes and alcohols), polyethylene glycol type phases are best suited - SolGel-WAX™, BP20 (WAX) and BP21(FFAP).

2. Internal Diameter

- The smaller the diameter the greater the efficiency, hence better resolution. Fast columns (0.1 mm ID) are used for faster analysis because the same resolution can be achieved in a shorter time.

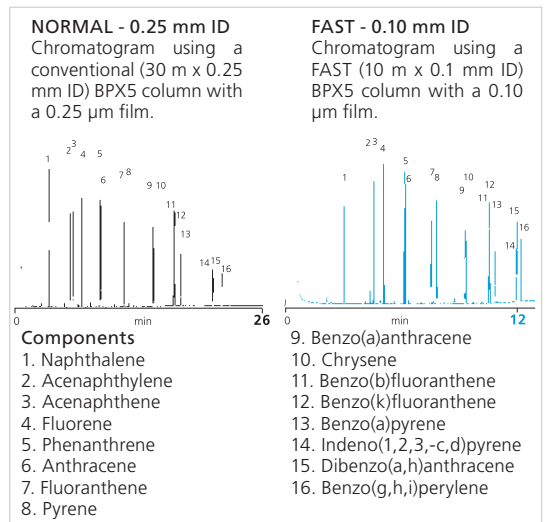

Effect of Internal Diameter. Polynuclear Aromatic Hydrocarbon (PAH) analysis.

3. Film Thickness

- For samples with a variation in solute concentration, a thicker film column is recommended. This will reduce the possibility of broad overloaded peaks co-eluting with other compounds of interest. If the separation of two solutes is sufficient and co-elution is still unlikely, even with large differences in concentration, then a thinner film can be used.
- The greater the film thickness the greater the retention of solutes, therefore the higher the elution temperature. As a rule, doubling the film thickness results in an increase in elution temperature of approximately 15-20 °C under isothermal conditions. Using a temperature program, the increase in elution temperature is slightly less.
- From the phase ratio value β , a column can be categorized for the type of application it would best suit. The smaller the β value, the greater the ratio of phase to the column inner diameter, making it better suited for analyzing volatile compounds.

Columns that have thin films are generally better suited for high molecular weight compounds and are characterized by large β values.

- Maintain phase ratio among different ID columns to yield similar chromatography.

$$\beta = \frac{id}{4d_f}$$


where

β = phase ratio

id = column internal diameter (μm)

d_f = film thickness (μm)

Formula to calculate Phase Ratio.

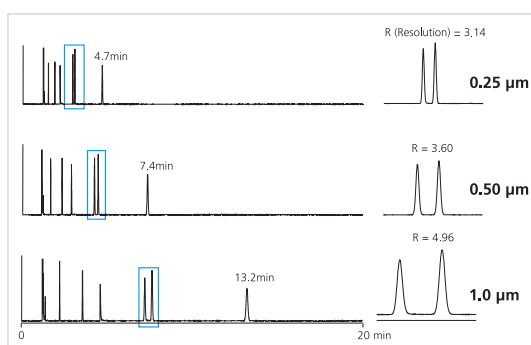


Effect of Film Thickness.

| Film Thickness (μm) | Column ID (μm) | | | | | |
|----------------------------------|-----------------------------|-----|-----|-----|-----|------|
| | 100 | 150 | 220 | 250 | 320 | 530 |
| 0.10 | 250 | - | 550 | 625 | 800 | 1325 |
| 0.15 | - | 250 | - | - | - | 883 |
| 0.25 | - | 150 | 220 | 250 | 320 | 530 |
| 0.50 | - | 75 | 110 | 125 | 160 | 265 |
| 1.00 | - | - | 55 | 63 | 80 | 132 |
| 3.00 | - | - | - | - | 27 | 44 |
| 5.00 | - | - | - | - | 16 | 26 |

Table 1. Above shows the phase ratio (β) available for the SGE range of capillary columns. Keeping a similar phase ratio when changing column internal diameters will ensure that your chromatographic parameters will not need substantial changes.

4. Column Length

- Always try to select the shortest column length that will provide the required resolution for the application. If the maximum column length available is being used and resolution of the sample mixture is still inadequate then try changing the stationary phase or internal diameter.
- Resolution is proportional to the square root of the column efficiency; therefore, doubling the column length will only increase the resolving power of the column by approximately 40%.

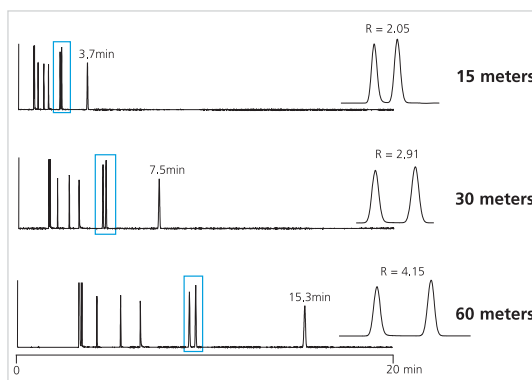

Effect of Length.



Application Range For Varying Phase Ratios

| Phase Ratio (β) | Application |
|-------------------------|--|
| 16-100 | Gases, Low M.W. Hydrocarbons, Solvents, Volatile Halogens (M.W.16-250) |
| 100-320 | Semi-volatiles, General Applications (M.W. 100-700) |
| 320-1325 | High M.W. Hydrocarbons, Waxes, Petroleum Products (M.W. 300-1500) |


GC Columns and Applications

SGE GC Capillary Column Phase Cross Reference Table

| SGE Phase | Description | Capillary Column to Replace |
|----------------------|---|--|
| BP1 | 100% Dimethyl Polysiloxane | DB-1, HP-1, Ultra-1, SPB-1, CP-Sil 5CB, RSL-150, RSL-160, Rtx [®] -1, ZB-1, CB-1, OV [®] -1, PE-1, 007-1(MS), SP-2100, SE-30, RH-1, CC-1, CP-Sil 5CB MS, VF-1ms, Petrocol DH |
| BP1-PONA | 100% Dimethyl Polysiloxane | Petrocol DH, DB-Petro |
| BPX1 | 100% Dimethyl Polysiloxane | DB-HT Sim Dis, DB-2887, Rtx-2887, HP-1, Petrocol 2887, Petrocol EX2887 |
| SolGel-1ms™ | SolGel + 100% Dimethyl Polysiloxane | Unique highly inert phase |
| BP5 | 5% Phenyl Polysiloxane | DB-5, DB-5.625, Rtx-5, HP-5, Ultra-2, PTE-5, PB-5, MDN-5, CP-Sil 8CB, VB-5 & ZB-5 |
| BPX5 | 5% Phenyl Polysilphenylene-siloxane | DB-5, DB-5ms, HP-5, Ultra-2, Rtx [®] -5, Rtx-5Sil MS, Rtx 5MS, AT-5, AT-5MS, 007-5MS, SPB-5,CP-Sil 8CB, VF-5ms, RSL-200, CB-5, OV [®] -5, PE-5, 007-2(MPS-5), SE-52, SE-54, XTI-5, PTE-5, CC-5, RH-5ms, ZB-5 |
| BPX35 | 35% Phenyl Polysilphenylene-siloxane | DB-35, DB-35ms, Rtx-35, HP-35, HP-35MS, SPB-35, MDN-35, VB-50, ZB-35 |
| BPX608 | 35% Phenyl Polysilphenylene-siloxane | DB-608, Rtx-35, SPB-608 |
| BPX50 | 50% Phenyl Polysilphenylene-siloxane | OV-17, SP-2250, DB-17ms, DB-17ht, Rtx-50, SPB-50, HP-50+, HP-17, VB-50/608, ZB-50 |
| HT5 | 5% Phenyl Polycarborane-siloxane | MXT-1 SimDist, HT-SimDist, DistCB, MXT-500 |
| HT8 | 8% Phenyl Polycarborane-siloxane | No equivalent, unique high temperature capillary column with special selectivity (standard for PCB) |
| BP225 | 50% Cyanopropylphenyl Polysiloxane | HP-225, DB-225, Rtx-225 |
| BP10 (1701) | 14% Cyanopropylphenyl Polysiloxane | DB-1701, Rtx-1701, HP-1701, SPB-7, CP-Sil 19CB, VB-1701, ZB-1701 |
| BP624, BPX-Volatiles | Cyanopropylphenyl Polysiloxane | DB-624, HP-VOC, Rtx Volatiles, Rtx 624, VOCOL, VB-624, ZB-624 |
| BPX70 | 70% Cyanopropyl Polysilphenylene-siloxane | DB-23, CP-Sil 88, VF-23ms, SP-2330, SP-2380, Rtx [®] -2330, 007-23, AT-Silar, PE-23 |
| BPX90 | 90% Cynopropyl Polysilphenylene-siloxane | Unique highly polar phase |
| BP21 (FFAP) | Polyethylene Glycol (TPA treated) | DB-FFAP, HP-FFAP, Stabilwax-DA, CP Wax 58CB, VB-FFAP, ZB-FFAP |
| BP20 (Wax) | Polyethylene Glycol | DB-Wax, Rtx-Wax, Stabilwax, HP20M, HP-Wax, HP-INNOWax, Supelcowax-10, AT-Wax, Nukol, CP Wax 2CB, VB-WAX, ZB-WAX |
| SolGel-WAX™ | SolGel + Polyethylene Glycol | Unique highly inert phase |
| CYDEX-B | Permethyated Beta Cyclodextrin | Cyclodex-B, Rt-BDEXm |

Operating Temperature


For each SGE GC column phases temperature limits are represented three ways:

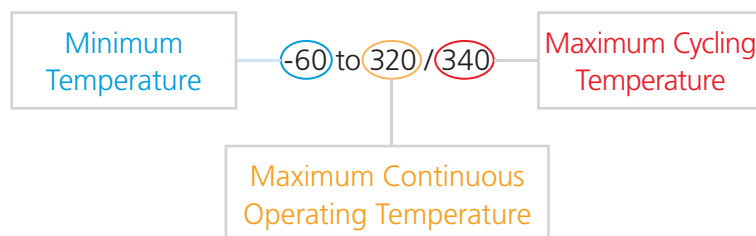

| Minimum Temperature | Maximum Continuous Operating Temperature | Maximum Cycling Temperature |
|--|--|--|
| The temperature below which the capillary column will not separate components due to loss of partitioning in the stationary phase. | The maximum temperature at which a capillary column can be held for 72 hours with no significant change. SGE capillary columns are designed to pass all criteria measured by their test analysis after 72 hours at their Maximum Continuous Operating Temperature. | The maximum cycling temperature to which a capillary column can be taken for short periods (up to 30 minutes) without causing serious bleed problems or degradation of the phase. This is usually higher than the Maximum Continuous Operating Temperature. The lifetime of a capillary column is affected by the amount of time it spends at high temperatures. |

BP1

- Classic crosslinked dimethyl polysiloxane technology.
- Excellent general purpose GC column.
- Low bleed.
- Non-polar.
- Suitable for all routine analyses.
- 320 – 340 °C upper temperature limit – dependent on film thickness.






GC Columns and Applications

Expert Tip :

Columns should be conditioned to the maximum continuous temperature unless specified.




| | |
|---|---|
| Especially Suitable for these Industries: |  Fuels  Environment  Forensics |
| Application Areas: | Suitable for analysis of hydrocarbons, aromatics, pesticides, phenol, herbicides, amines. Applications AMI04, POL05, PHA04. |
| Suitable Replacement for: | DB-1, DB-Petro, HP-1, HP-1MS, Rtx-1, Ultra-1, SPB-1, SPB-1 Sulfur, Petrocol DH, CP-Sil 5CB, VB-1, ZB-1, VF-1ms. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.1 | 10 | -60 to 320/340 | 054022 |
| 0.15 | 0.25 | 12 | -60 to 320/340 | 054028 |
| 0.15 | 0.25 | 25 | -60 to 320/340 | 054029 |
| 0.22 | 0.1 | 12 | -60 to 320/340 | 054040 |
| 0.22 | 0.25 | 12 | -60 to 320/340 | 054046 |
| 0.22 | 1 | 12 | -60 to 320/340 | 054052 |
| 0.22 | 0.25 | 15 | -60 to 320/340 | 054049 |
| 0.22 | 0.1 | 25 | -60 to 320/340 | 054041 |
| 0.22 | 0.25 | 25 | -60 to 320/340 | 054047 |
| 0.22 | 1 | 25 | -60 to 320/340 | 054053 |
| 0.22 | 0.25 | 30 | -60 to 320/340 | 054050 |
| 0.22 | 0.1 | 50 | -60 to 320/340 | 054042 |
| 0.22 | 0.25 | 50 | -60 to 320/340 | 054048 |
| 0.22 | 1 | 50 | -60 to 320/340 | 054054 |
| 0.22 | 0.25 | 60 | -60 to 320/340 | 054051 |
| 0.25 | 0.1 | 15 | -60 to 320/340 | 054039 |
| 0.25 | 0.25 | 15 | -60 to 320/340 | 054043 |
| 0.25 | 0.25 | 30 | -60 to 320/340 | 054044 |
| 0.25 | 0.5 | 30 | -60 to 320/340 | 054820 |
| 0.25 | 1 | 30 | -60 to 320/340 | 054056 |
| 0.25 | 0.25 | 60 | -60 to 320/340 | 054045 |
| 0.25 | 0.5 | 60 | -60 to 320/340 | 054812 |
| 0.25 | 1 | 60 | -60 to 320/340 | 054815 |
| 0.32 | 0.25 | 12 | -60 to 320/340 | 054058 |
| 0.32 | 0.5 | 12 | -60 to 320/340 | 054064 |
| 0.32 | 1 | 12 | -60 to 320/340 | 054070 |
| 0.32 | 0.25 | 15 | -60 to 320/340 | 054061 |
| 0.32 | 0.25 | 25 | -60 to 320/340 | 054059 |
| 0.32 | 0.5 | 25 | -60 to 320/340 | 054065 |
| 0.32 | 1 | 25 | -60 to 320/340 | 054071 |
| 0.32 | 4 | 25 | -60 to 280/300 | 054076 |
| 0.32 | 5 | 25 | -60 to 280/300 | 054081 |
| 0.32 | 0.25 | 30 | -60 to 320/340 | 054062 |
| 0.32 | 0.5 | 30 | -60 to 320/340 | 054068 |
| 0.32 | 1 | 30 | -60 to 320/340 | 054813 |
| 0.32 | 1.5 | 30 | -60 to 300/320 | 054811 |
| 0.32 | 3 | 30 | -60 to 300/320 | 054073 |
| 0.32 | 4 | 30 | -60 to 280/300 | 054077 |
| 0.32 | 0.25 | 50 | -60 to 320/340 | 054060 |
| 0.32 | 0.5 | 50 | -60 to 320/340 | 054066 |
| 0.32 | 1 | 50 | -60 to 320/340 | 054072 |
| 0.32 | 5 | 50 | -60 to 280/300 | 054082 |
| 0.32 | 0.25 | 60 | -60 to 320/340 | 054067 |




GC Columns and Applications

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.32 | 0.5 | 60 | -60 to 320/340 | 054069 |
| 0.32 | 1 | 60 | -60 to 320/340 | 054810 |
| 0.32 | 5 | 60 | -60 to 280/300 | 054085 |
| 0.53 | 1 | 12 | -60 to 320/340 | 054086 |
| 0.53 | 3 | 12 | -60 to 300/320 | 054097 |
| 0.53 | 0.5 | 15 | -60 to 320/340 | 054870 |
| 0.53 | 1 | 15 | -60 to 320/340 | 054089 |
| 0.53 | 1 | 25 | -60 to 320/340 | 054087 |
| 0.53 | 3 | 25 | -60 to 300/320 | 054098 |
| 0.53 | 5 | 25 | -60 to 280/300 | 054095 |
| 0.53 | 0.5 | 30 | -60 to 320/340 | 054092 |
| 0.53 | 1 | 30 | -60 to 320/340 | 054090 |
| 0.53 | 2.6 | 30 | -60 to 300/320 | 054819 |
| 0.53 | 3 | 30 | -60 to 300/320 | 054808 |
| 0.53 | 5 | 30 | -60 to 280/300 | 054806 |
| 0.53 | 1 | 50 | -60 to 320/340 | 054088 |
| 0.53 | 5 | 50 | -60 to 280/300 | 054096 |
| 0.53 | 0.5 | 60 | -60 to 320/340 | 054871 |
| 0.53 | 3 | 60 | -60 to 300/320 | 054809 |
| 0.53 | 5 | 60 | -60 to 280/300 | 054807 |




BP1 PONA

- Designed for the analysis of petroleum products.
- Non-polar phase for PONA analysis.
- Detailed hydrocarbon analysis according to ASTM (DHA-method).
- Crosslinked and washable.
- Very high resolving power columns for complex samples.
- 320 – 340 °C upper temperature limit.


| | |
|--|---|
| Especially Suitable for this Industry: |  Fuels |
| Application Areas: | Suitable for petroleum hydrocarbons, gasoline range hydrocarbons, MTBE, paraffins, olefins, naphthenes, aromatics. Application PET01. |
| Suitable Replacement for: | Petrocol DH, DB-Petro, HP-PONA, AT-Petro, Elite-PONA, ZB-1, 007-1-100-0.5F, Rtx-1PONA, CP Sil PONA. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.15 | 0.5 | 50 | -60 to 320/340 | 054950 |
| 0.25 | 0.5 | 100 | -60 to 320/340 | 054818 |



BPX1

- Non-polar column.
- Dimensionally stabilized phase.
- Low bleed.
- Specifically designed for high temperature hydrocarbon analysis.
- Ideal for simulated distillation methods (ASTM Method D2887).
- 430 °C upper temperature limit – Aluminum clad.
- 370- 400 °C upper temperature limit – Polyimide clad (dependent on film thickness).

| | |
|--|--|
| Especially Suitable for this Industry: |  Fuels |
| Application Areas: | ASTM methods D2887 and D6532. Applications PET26, PET18, ENV54. |
| Suitable Replacement for: | DB-2887, DB-HT Sim Dis, HP-1, Petrocol 2887, Petrocol EX2887, Rtx-2887. |

BPX1

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|-----------------------|---------------------|------------|-------------------------|----------|
| Polyimide Clad | | | | |
| 0.1 | 0.1 | 10 | -30 to 400/400 | 054777 |
| 0.53 | 2.65 | 6 | -30 to 370/370 | 0548025 |
| 0.53 | 0.1 | 10 | -30 to 400/400 | 054803 |
| 0.53 | 0.9 | 10 | -30 to 400/400 | 054801 |
| 0.53 | 2.65 | 10 | -30 to 370/370 | 054802 |
| Aluminum Clad | | | | |
| 0.53 | 0.1 | 5 | -30 to 430/430 | 054800 |
| 0.53 | 0.17 | 5 | -30 to 430/430 | 054782 |
| 0.53 | 0.1 | 10 | -30 to 430/430 | 054779 |


GC Columns and Applications

GC Capillary Columns | 100% Dimethyl Polysiloxane in a Sol-Gel Matrix

SolGel-1ms™

What is Sol-Gel?

Sol-Gel is essentially a synthetic glass with ceramic-like properties. These modified Sol-Gels offer the best of both worlds – ceramic-like properties with the film-forming properties of the associated polymer. The Sol-Gel process involves hydrolysis and condensation of alkoxides that lead to the formation of a glassy material at ambient temperatures. This method has been used to produce high quality ceramics and mono- and multi-component glasses of high homogeneity and purity. The further modification of this ceramic material with polymeric material (with appropriate functionality) leads to the formation of organic-inorganic nanomaterials.

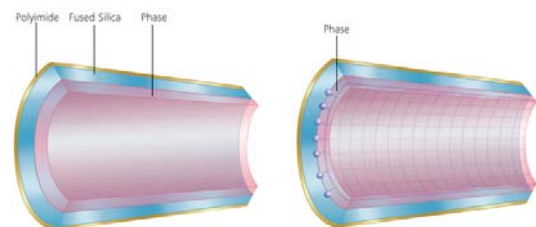

Conventional Phase
The phase is coated onto the surface of the fused silica resulting in weak intermolecular bonding but no covalent bonding, ie no anchoring.


Sol-Gel Phase
Anchored to the surface of the fused silica through covalent bonding.

Where can Sol-Gel materials be used?

The further organic-modified Sol-Gels have been incorporated in a variety of high-end technology products including membrane chemical and pH sensors, films for protection of optical lenses, cosmetic and electronic products.

SGE and Sol-Gel materials?

At SGE, Sol-Gel processes are used to manufacture stationary phases for gas chromatography capillary columns. SGE is the first company to offer Sol-Gel technology capillary columns. The organic component in our case is a GC stationary phase. The final Sol-Gel product has all the properties of the GC phase as well as the additional properties of the Sol-Gel part. The Sol-Gel material is able to covalently bond to the surface of the fused silica. The 'heavy-duty' bonding imparts better thermal stability of the phase leading to ultra-low bleed capillary columns. To date, two Sol-Gel phases have been developed by SGE, namely SolGel-1ms™ and SolGel-WAX™. The SolGel-1ms™ stationary phase is a non-polar phase derived from 100% dimethyl polysiloxane. SolGel-WAX™ is a polar phase which incorporates polyethylene glycol in the matrix.



Expert Tip :




Always use SilTite™ or SilTite™ Finger-Tite ferrules when connecting a column to a GC/MS interface.



SolGel-1ms™ has a robust, inert, high temperature, non-polar phase for use with mass spectrometers.


- Highly inert.
- Less bleed means:
 - Better MS library identification.
 - Less ion source maintenance.
 - Better sensitivity.
- Can also be used for all non-MS detectors.
- Same selectivity as BP1.
- 340 /360 °C upper temperature limit.

GC Columns and Applications

| | |
|---|---|
| Especially Suitable for these Industries: |    |
| Application Areas: | Recommended for highly active compounds. Applications ARO14, ENV51. |
| Operating Temperature: | 0.25 µm film thickness 0 °C to 340/360 °C. |
| Suitable Replacement for: | DB-1, DB-Petro, HP-1, HP-1MS, Rtx-1, Ultra-1, SPB-1, SPB-1 Sulfur, Petrocol DH, CP-Sil 5CB, VB-1, ZB-1, VF-1ms. |


| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.25 | 0.25 | 30 | 0 to 340/360 | 054795 |
| 0.25 | 0.25 | 60 | 0 to 340/360 | 054793 |
| 0.32 | 0.25 | 30 | 0 to 340/360 | 054798 |
| 0.32 | 0.25 | 60 | 0 to 340/360 | 054794 |

GC Capillary Columns | 5% Phenyl / 95% Dimethyl Polysiloxane



BP5

- Excellent general purpose GC column.
- Low bleed.
- Non-polar.
- High temperature.
- 320/340 °C upper temperature limit - dependent on film thickness.

| | |
|---|--|
| Especially Suitable for these Industries: |  All Industries |
| Application Areas: | General purpose, aromatics, pesticides, herbicides, drugs of abuse, hydrocarbons, solvent impurities, PCB congeners or Aroclor mixes, essential oils, semivolatiles. Applications FOO02, AMI03, PHA08, PHA 10. |
| Suitable Replacement for: | DB-5, Rtx-5, HP-5, Ultra-2, PTE-5, SPB-5, MDN-5, CP-Sil 8CB, VB-5, ZB-5. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.22 | 0.25 | 12 | -60 to 320/340 | 054167 |
| 0.22 | 0.25 | 25 | -60 to 320/340 | 054168 |
| 0.22 | 0.25 | 30 | -60 to 320/340 | 054171 |
| 0.22 | 0.25 | 50 | -60 to 320/340 | 054169 |
| 0.22 | 1 | 50 | -60 to 320/340 | 054175 |
| 0.25 | 0.25 | 15 | -60 to 320/340 | 054182 |
| 0.25 | 0.25 | 30 | -60 to 320/340 | 054183 |
| 0.25 | 0.5 | 30 | -60 to 320/340 | 054202 |
| 0.25 | 1 | 30 | -60 to 320/340 | 054203 |

BP5

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.25 | 0.25 | 60 | -60 to 320/340 | 054184 |
| 0.25 | 1 | 60 | -60 to 320/340 | 054215 |
| 0.32 | 0.25 | 12 | -60 to 320/340 | 054179 |
| 0.32 | 0.25 | 15 | -60 to 320/340 | 054176 |
| 0.32 | 0.25 | 25 | -60 to 320/340 | 054180 |
| 0.32 | 0.5 | 25 | -60 to 320/340 | 054186 |
| 0.32 | 1 | 25 | -60 to 320/340 | 054192 |
| 0.32 | 0.25 | 30 | -60 to 320/340 | 054177 |
| 0.32 | 0.5 | 30 | -60 to 320/340 | 054216 |
| 0.32 | 1 | 30 | -60 to 320/340 | 054189 |
| 0.32 | 0.5 | 50 | -60 to 320/340 | 054187 |
| 0.32 | 1 | 50 | -60 to 320/340 | 054193 |
| 0.32 | 0.25 | 60 | -60 to 320/340 | 054178 |
| 0.32 | 1 | 60 | -60 to 320/340 | 054188 |
| 0.53 | 1 | 12 | -60 to 320/340 | 054197 |
| 0.53 | 1 | 15 | -60 to 320/340 | 054194 |
| 0.53 | 1.5 | 15 | -60 to 320/340 | 054199 |
| 0.53 | 1 | 25 | -60 to 320/340 | 054198 |
| 0.53 | 0.5 | 30 | -60 to 320/340 | 0541935 |
| 0.53 | 1 | 30 | -60 to 320/340 | 054195 |
| 0.53 | 5 | 30 | -60 to 280/300 | 054196 |
| 0.53 | 1.5 | 60 | -60 to 280/300 | 054204 |

GC Columns and Applications

Expert Tip :


If the injection port temperature is not specified in the method, 250 °C is usually the recommended temperature.




GC Capillary Columns | 5% Phenyl Polysilphenylene-siloxane

BPX5

- High temperature.
- General purpose GC column – suitable for over 80% of all routine analyses performed by gas chromatography.
- Very low bleed – ideal for trace analysis.
- Non-polar.
- Extremely inert.
- Ideal for GC-MS.
- 360 – 370 °C upper temperature limit – dependent on film thickness.

| | |
|---|---|
| Especially Suitable for these Industries: |  All Industries |
| Areas: | Ultra trace analyses, pesticides/herbicides, hydrocarbons, solvents, phenols, amines, GC/MS and other specific detector applications. Applications ENV62, ARO09, ENV20, ENV03, ENV48, ENV59, ENV84, FOO21, FLA14, FLA16, FLA15, FLA12 FLA13, ENV54, PET22, SOL33 PHA06, PHA08, PHA15. |
| Suitable Replacement for: | DB-5, DB-5ms, DB-5.625, XTI-5, Rtx-5ms, Ultra-2, HP-5, HP-5MS, HP5-TA, SPB-5, MDN-5S, CP-Sil8CB, Rxt-Sil 5MS, AT-5ms, VB-5, ZB-5, VF-5ms. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.1 | 10 | -40 to 360/370 | 054099 |
| 0.15 | 1.2 | 10 | -40 to 360/370 | 054106 |
| 0.15 | 0.25 | 12 | -40 to 360/370 | 054103 |
| 0.15 | 0.4 | 12 | -40 to 360/370 | 054107 |
| 0.15 | 0.25 | 25 | -40 to 360/370 | 054104 |
| 0.15 | 0.4 | 25 | -40 to 360/370 | 054108 |




BPX5

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.15 | 0.15 | 30 | -40 to 360/370 | 054110 |
| 0.15 | 0.25 | 50 | -40 to 360/370 | 054105 |
| 0.18 | 0.18 | 40 | -40 to 360/370 | 054229 |
| 0.22 | 0.25 | 12 | -40 to 360/370 | 054112 |
| 0.22 | 0.25 | 25 | -40 to 360/370 | 054113 |
| 0.22 | 1 | 25 | -40 to 360/370 | 054116 |
| 0.22 | 0.25 | 30 | -40 to 360/370 | 054142 |
| 0.22 | 0.25 | 50 | -40 to 360/370 | 054114 |
| 0.22 | 1 | 50 | -40 to 360/370 | 054117 |
| 0.25 | 0.25 | 7 | -40 to 360/370 | 054149 |
| 0.25 | 0.1 | 15 | -40 to 360/370 | 0542170 |
| 0.25 | 0.25 | 15 | -40 to 360/370 | 054100 |
| 0.25 | 1 | 15 | -40 to 360/370 | 054121 |
| 0.25 | 0.1 | 30 | -40 to 360/370 | 0541011 |
| 0.25 | 0.25 | 30 | -40 to 360/370 | 054101 |
| 0.25 | 0.5 | 30 | -40 to 360/370 | 0541025 |
| 0.25 | 1 | 30 | -40 to 360/370 | 054122 |
| 0.25 | 0.25 | 60 | -40 to 360/370 | 054102 |
| 0.25 | 1 | 60 | -40 to 360/370 | 054123 |
| 0.32 | 1 | 6 | -40 to 360/370 | 0541261 |
| 0.32 | 0.25 | 12 | -40 to 360/370 | 054118 |
| 0.32 | 0.5 | 12 | -40 to 360/370 | 054124 |
| 0.32 | 1 | 12 | -40 to 360/370 | 054127 |
| 0.32 | 0.25 | 15 | -40 to 360/370 | 054144 |
| 0.32 | 1 | 15 | -40 to 360/370 | 054152 |
| 0.32 | 0.25 | 25 | -40 to 360/370 | 054119 |
| 0.32 | 0.5 | 25 | -40 to 360/370 | 054125 |
| 0.32 | 1 | 25 | -40 to 360/370 | 054128 |
| 0.32 | 3 | 25 | -40 to 350/360 | 054136 |
| 0.32 | 0.25 | 30 | -40 to 360/370 | 054145 |
| 0.32 | 0.5 | 30 | -40 to 360/370 | 0541205 |
| 0.32 | 1 | 30 | -40 to 360/370 | 054153 |
| 0.32 | 0.25 | 50 | -40 to 360/370 | 054120 |
| 0.32 | 0.5 | 50 | -40 to 360/370 | 054126 |
| 0.32 | 1 | 50 | -40 to 360/370 | 054129 |
| 0.32 | 0.25 | 60 | -40 to 360/370 | 054146 |
| 0.32 | 1 | 60 | -40 to 360/370 | 054154 |
| 0.53 | 0.25 | 12 | -40 to 360/370 | 054133 |
| 0.53 | 1 | 12 | -40 to 360/370 | 054130 |
| 0.53 | 3 | 12 | -40 to 350/360 | 054138 |
| 0.53 | 0.5 | 15 | -40 to 360/370 | 0541344 |
| 0.53 | 1 | 15 | -40 to 360/370 | 054147 |
| 0.53 | 1.5 | 15 | -40 to 350/360 | 0541347 |
| 0.53 | 3 | 15 | -40 to 350/360 | 054159 |
| 0.53 | 0.25 | 25 | -40 to 360/370 | 054134 |
| 0.53 | 1 | 25 | -40 to 360/370 | 054131 |
| 0.53 | 3 | 25 | -40 to 350/360 | 054139 |
| 0.53 | 0.5 | 30 | -40 to 360/370 | 0541345 |
| 0.53 | 1 | 30 | -40 to 360/370 | 054148 |
| 0.53 | 1.5 | 30 | -40 to 350/360 | 0541348 |
| 0.53 | 3 | 30 | -40 to 350/360 | 054160 |
| 0.53 | 1 | 50 | -40 to 360/370 | 054132 |
| 0.53 | 1 | 60 | -40 to 360/370 | 054158 |


GC Columns and Applications

Expert Tip :

If you're having problems with solvent focusing, or early eluting peaks seem broad or lop-sided in splitless injection, then try using a column with a thicker film.

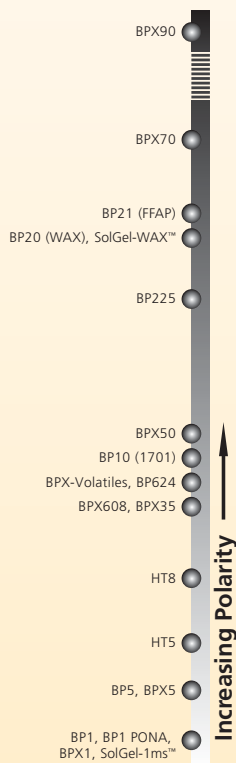




HT5



GC Columns and Applications

- Ultra high temperature columns.
- Unique phase – no equivalent phases.
- Ideal for simulated distillation applications (petroleum industry).
- 460/480 °C upper temperature limit – Aluminum clad.
- 380/400 °C upper temperature limit – Polyimide clad.
- Bonded and cross-linked.
- Able to be solvent rinsed.


| | |
|---|--|
| Especially Suitable for these Industries: |  Fuels  Environment  Food |
| Application Areas: | Simulated distillation, general hydrocarbon profiles, pesticides/herbicides, GC/MS applications. Applications FOO16, PET11, PET27, PET06. |
| Suitable Replacement for: | MXT-1 Sim Dist, HT-Sim, DistCB, MXT-500. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|-----------------------|---------------------|------------|-------------------------|----------|
| Polyimide Clad | | | | |
| 0.22 | 0.1 | 12 | 10 to 380/400 | 054631 |
| 0.22 | 0.1 | 25 | 10 to 380/400 | 054632 |
| 0.25 | 0.1 | 15 | 10 to 380/400 | 054633 |
| 0.25 | 0.1 | 30 | 10 to 380/400 | 054634 |
| 0.32 | 0.1 | 12 | 10 to 380/400 | 054641 |
| 0.32 | 0.5 | 15 | 10 to 380/400 | 054667 |
| 0.32 | 0.1 | 25 | 10 to 380/400 | 054642 |
| 0.32 | 0.5 | 30 | 10 to 380/400 | 054668 |
| 0.53 | 0.1 | 6 | 10 to 380/400 | 054655 |
| 0.53 | 0.5 | 10 | 10 to 380/400 | 054670 |
| 0.53 | 0.15 | 12 | 10 to 380/400 | 054657 |
| 0.53 | 0.5 | 15 | 10 to 380/400 | 054671 |
| 0.53 | 0.15 | 25 | 10 to 380/400 | 054658 |
| 0.53 | 0.5 | 30 | 10 to 380/400 | 054672 |
| Aluminum Clad | | | | |
| 0.22 | 0.1 | 12 | 10 to 460/480 | 054635 |
| 0.22 | 0.1 | 25 | 10 to 460/480 | 054636 |
| 0.32 | 0.1 | 12 | 10 to 460/480 | 054651 |
| 0.32 | 0.1 | 25 | 10 to 460/480 | 054652 |
| 0.32 | 0.1 | 50 | 10 to 460/480 | 054653 |
| 0.53 | 0.075 | 5 | 10 to 460/480 | 054673 |
| 0.53 | 0.1 | 6 | 10 to 460/480 | 054661 |
| 0.53 | 0.15 | 12 | 10 to 460/480 | 054662 |
| 0.53 | 0.15 | 25 | 10 to 460/480 | 054665 |

Expert Tip :

To prevent increasing retention times in your chromatography, replace the septum regularly.







HT8

- High temperature.
- Low bleed.
- Preferred column for polychlorinated biphenyl (PCB) compounds.
- Separates PCB's on ortho ring substitution as well as boiling point.
- Ideal for environmental analysis.
- 360/370 °C upper temperature limit.
- Unique high temperature phase suited for the analysis of persistent organic pollutants (POPs).


GC Columns and Applications

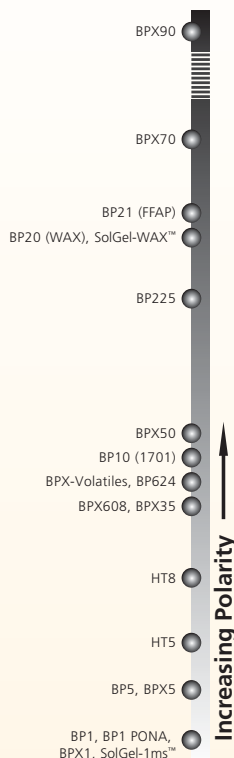

| | |
|--|--|
| Especially Suitable for this Industry: |  Environment |
| Application Areas: | PCB congener analyses, nitro-substituted aromatics, polynuclear aromatic hydrocarbons, pesticides/herbicides. Application ARO08. |
| Suitable Replacement for: | No equivalents, unique ultra high temperature column. |





| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.1 | 10 | -20 to 360/370 | 054690 |
| 0.22 | 0.25 | 12 | -20 to 360/370 | 054674 |
| 0.22 | 0.25 | 25 | -20 to 360/370 | 054675 |
| 0.22 | 0.25 | 50 | -20 to 360/370 | 054676 |
| 0.25 | 0.25 | 30 | -20 to 360/370 | 054677 |
| 0.25 | 0.25 | 60 | -20 to 360/370 | 054683 |
| 0.32 | 0.25 | 12 | -20 to 360/370 | 054679 |
| 0.32 | 0.25 | 25 | -20 to 360/370 | 054680 |
| 0.32 | 0.25 | 50 | -20 to 360/370 | 054681 |
| 0.32 | 0.25 | 60 | -20 to 360/370 | 054682 |
| 0.53 | 0.5 | 12 | -20 to 360/370 | 054684 |
| 0.53 | 0.5 | 25 | -20 to 360/370 | 054685 |

GC Capillary Columns | 35% Phenyl Polysilphenylene-siloxane



BPX35

- Mid polarity column.
- Ideal for confirmational analysis.
- Inert.
- Equivalent to USP phase G42.
- High temperature.
- Very low bleed.
- Pharmaceutical specialist.
- 330/360 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

| | |
|---|---|
| Especially Suitable for these Industries: |     Pharmaceuticals Environment Food Forensics |
| Application Areas: | Environmental analyses, pesticides/herbicides, drugs of abuse, pharmaceuticals, polynuclear aromatic hydrocarbons, GC/MS applications. Applications ENV57, ENV04 AMI09, ALC09, SOL25, PHA14, PHA09 |
| Suitable Replacement for: | DB-35, DB-35ms, Rtx-35, HP-35, HP-35MS, SPB-35, MDN-35. |

BPX35

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.1 | 10 | 10 to 330/360 | 054699 |
| 0.22 | 0.25 | 15 | 10 to 330/360 | 054713 |
| 0.22 | 0.25 | 25 | 10 to 330/360 | 054711 |
| 0.22 | 0.25 | 30 | 10 to 330/360 | 054714 |
| 0.22 | 0.25 | 50 | 10 to 330/360 | 054712 |
| 0.25 | 0.25 | 15 | 10 to 330/360 | 054700 |
| 0.25 | 1 | 15 | 10 to 330/360 | 054703 |
| 0.25 | 0.25 | 30 | 10 to 330/360 | 054701 |
| 0.25 | 0.5 | 30 | 10 to 330/360 | 0547025 |
| 0.25 | 1 | 30 | 10 to 330/360 | 054704 |
| 0.25 | 0.25 | 60 | 10 to 330/360 | 054702 |
| 0.25 | 1 | 60 | 10 to 330/360 | 054705 |
| 0.32 | 0.25 | 15 | 10 to 330/360 | 054723 |
| 0.32 | 0.5 | 15 | 10 to 330/360 | 054718 |
| 0.32 | 1 | 15 | 10 to 330/360 | 054716 |
| 0.32 | 0.25 | 25 | 10 to 330/360 | 054721 |
| 0.32 | 0.25 | 30 | 10 to 330/360 | 054724 |
| 0.32 | 0.5 | 30 | 10 to 330/360 | 0547158 |
| 0.32 | 1 | 30 | 10 to 330/360 | 054717 |
| 0.32 | 0.25 | 50 | 10 to 330/360 | 054722 |
| 0.53 | 0.5 | 15 | 10 to 330/360 | 054734 |
| 0.53 | 1 | 15 | 10 to 330/360 | 054736 |
| 0.53 | 0.5 | 30 | 10 to 330/360 | 054735 |
| 0.53 | 1 | 30 | 10 to 330/360 | 054737 |

GC Columns and Applications

Expert Tip :


When peak shape deteriorates, replace the liner immediately and cut 30cm from the front end of the column.




GC Capillary Columns | 35% Phenyl Polysilphenylene-siloxane


BPX608

- Optimized for ECD.
- Ideal for organochlorine, pesticides and herbicides analysis.
- Maximum temperature 370 °C.

| | |
|---|--|
| Especially Suitable for these Industries: |  Environment |
| Application Areas: | Environmental analyses, EPA 608, pesticides/herbicides. |
| Operating Temperature | 10 °C to 360/370 °C. |
| Suitable Replacement for: | DB-608, Rtx-35, SPB-608, HP-35, ZB-35. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.32 | 0.4 | 25 | 10 to 360/370 | 054823 |





BPX50

- Mid polarity.
- Inert.
- Low bleed.
- High temperature.
- Ideal for a range of EPA methods and pharmaceutical applications.
- 330/350 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

GC Columns and Applications

Especially Suitable for these Industries:



Application Areas:

EPA methods 604, 608, 8060, 8081, triazines/herbicides, drug screening, steroids and a variety of pharmaceutical applications GC2D. Applications ENV62, ENV45, ENV65, PHA19.

Suitable Replacement for:

OV-17, SP-2250, DB-17, DB-17ms, DB-17ht, Rtx-50, SPB-50, HP-50+, HP-17.


Expert Tip :

When installing your column into an FID jet, never pass the column through the flame. This will burn the inner (phase) and outer (polyimide) coatings and will cause higher background signals.



| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.05 | 10 | 10 to 330/350 | 054739 |
| 0.1 | 0.07 | 10 | 10 to 330/350 | 054738 |
| 0.1 | 0.1 | 10 | 10 to 330/350 | 054740 |
| 0.15 | 0.15 | 30 | 10 to 330/350 | 054741 |
| 0.25 | 0.25 | 15 | 10 to 330/350 | 054750 |
| 0.25 | 0.25 | 30 | 10 to 330/350 | 054751 |
| 0.25 | 0.25 | 60 | 10 to 330/350 | 054752 |
| 0.32 | 0.25 | 15 | 10 to 330/350 | 054760 |
| 0.32 | 0.25 | 30 | 10 to 330/350 | 054761 |
| 0.32 | 0.25 | 60 | 10 to 330/350 | 054762 |
| 0.53 | 0.5 | 15 | 10 to 330/350 | 054770 |
| 0.53 | 0.5 | 30 | 10 to 330/350 | 054771 |
| 0.53 | 1.0 | 30 | 10 to 330/350 | 054772 |

GC Capillary Columns | 70% Cyanopropyl Polysilphenylene-siloxane



BPX70

- High temperature.
- Custom designed for separation of Fatty Acid Methyl Esters (FAMES).
- Industry standard column for FAME analysis.
- Polar phase.
- Long operating life.
- 250/260 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

Especially Suitable for these Industries:



Application Areas:

Fatty acid methyl esters (FAMES), carbohydrates, pharmaceuticals, GC/MS applications. Applications FOO02, FOO04.

Suitable Replacement for:

DB-23, Rtx-2330, SP-2330, CP-Sil 88, SP2380, HP-23.

BPX70

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.2 | 10 | 50 to 250/260 | 054600 |
| 0.22 | 0.25 | 12 | 50 to 250/260 | 054601 |
| 0.22 | 0.25 | 25 | 50 to 250/260 | 054602 |
| 0.22 | 0.25 | 30 | 50 to 250/260 | 054612 |
| 0.22 | 0.25 | 50 | 50 to 250/260 | 054603 |
| 0.22 | 0.25 | 60 | 50 to 250/260 | 054613 |
| 0.25 | 0.25 | 15 | 50 to 250/260 | 054621 |
| 0.25 | 0.25 | 30 | 50 to 250/260 | 054622 |
| 0.25 | 0.25 | 60 | 50 to 250/260 | 054623 |
| 0.25 | 0.25 | 120 | 50 to 250/260 | 054624 |
| 0.32 | 0.25 | 12 | 50 to 250/260 | 054605 |
| 0.32 | 0.25 | 25 | 50 to 250/260 | 054606 |
| 0.32 | 0.25 | 30 | 50 to 250/260 | 054616 |
| 0.32 | 0.25 | 50 | 50 to 250/260 | 054607 |
| 0.32 | 0.25 | 60 | 50 to 250/260 | 054617 |
| 0.53 | 0.5 | 15 | 50 to 250/260 | 054619 |
| 0.53 | 0.5 | 25 | 50 to 250/260 | 054610 |
| 0.53 | 0.5 | 30 | 50 to 250/260 | 054620 |

GC Columns and Applications

Expert Tip :





Set the FID temperature 20 °C above the maximum method temperature.




GC Capillary Columns | 90% Cyanopropyl Polysilphenylene-siloxane

BPX90

- Unique bonded phase.
- Highly polar.
- Thermally stable.
- Excellent resolution for cis and trans isomers.
- 260/280 °C upper temperature limit.
- Able to be solvent rinsed.

| | |
|---|---|
| Especially Suitable for these Industries: |     |
| Application Areas: | Ideal for fast separation of fragrances, aromatics, petrochemical, pesticides, PCBs and isomers of Fatty Acid Methyl Esters (FAMES). Application AN0022C. |
| Suitable Replacement for: | Unique to SGE. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.25 | 0.25 | 15 | 80 to 260/280 | 054570 |
| 0.25 | 0.25 | 30 | 80 to 260/280 | 054580 |
| 0.25 | 0.25 | 60 | 80 to 260/280 | 054590 |
| 0.25 | 0.25 | 100 | 80 to 260/280 | 054596 |
| 0.32 | 0.5 | 15 | 80 to 260/280 | 054573 |
| 0.32 | 0.5 | 30 | 80 to 260/280 | 054583 |
| 0.32 | 0.5 | 60 | 80 to 260/280 | 054593 |

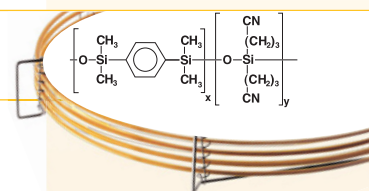



GC Capillary Columns | in a Sol-Gel matrix



SolGel-WAX™


GC Columns and Applications

- The world's highest temperature wax phase.
- Bonded polyethylene glycol.
- Very robust high-temperature column.
- Less susceptible to damage by oxygen than conventional wax phases.
- Polar phase.
- Low bleed and inert.
- 280 °C upper temperature limit.
- Bonded and cross-linked.
- Able to be solvent rinsed.

| | |
|---|---|
| Especially Suitable for these Industries: |   |
| Application Areas: | Recommended for highly active compounds. Applications ARO13, FLA19, FLA22, FLA21, FLA18, POL06, ENV52. |
| Suitable Replacement for: | DB-Wax, Rtx-Wax, Stabilwax, HP20M, HP-Wax, HP-INNOWax, Supelcowax-10, AT-Wax, Nukol, CP Wax 52CB, VB-WAX, ZB-WAX. |




| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.1 | 10 | 30 to 260/280 | 0547100 |
| 0.25 | 0.25 | 30 | 30 to 260/280 | 054796 |
| 0.25 | 1 | 30 | 30 to 260/280 | 054787 |
| 0.25 | 0.25 | 60 | 30 to 260/280 | 054791 |
| 0.32 | 0.25 | 30 | 30 to 260/280 | 054788 |
| 0.32 | 0.5 | 30 | 30 to 260/280 | 054797 |
| 0.32 | 0.25 | 60 | 30 to 260/280 | 054789 |
| 0.32 | 0.5 | 60 | 30 to 260/280 | 054792 |
| 0.53 | 0.5 | 30 | 30 to 260/280 | 054786 |
| 0.53 | 1 | 30 | 30 to 260/280 | 054785 |

GC Capillary Columns | Polyethylene Glycol



BP20 (WAX)


- Industry standard wax column.
- Polar phase.
- 240 – 280 °C upper temperature limit – dependent on film thickness.
- Bonded and cross-linked.
- Able to be solvent rinsed.

| | |
|---|---|
| Especially Suitable for these Industries: |    |
| Application Areas: | Alcohol, free acids, fatty acid methyl esters (FAMES), aromatics, solvents, essential oils. Applications FOO03, FOO24 FLA03, ALC03, ACI03, POL01, PHA13. |
| Suitable Replacement for: | DB-Wax, HP-20M, Supelcowax 10, CB-Wax, Stabilwax, Carbowax, HP-Innowax, Rtx-WAX, PE-WAX, RH-WAX, ZB-WAX, TRWAX. |

BP20 (WAX)

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.1 | 0.1 | 10 | 20 to 260/280 | 054405 |
| 0.22 | 0.25 | 12 | 20 to 260/280 | 054420 |
| 0.22 | 0.25 | 25 | 20 to 260/280 | 054421 |
| 0.22 | 0.25 | 30 | 20 to 260/280 | 054424 |
| 0.22 | 0.25 | 50 | 20 to 260/280 | 054422 |
| 0.22 | 0.25 | 60 | 20 to 260/280 | 054425 |
| 0.25 | 0.25 | 15 | 20 to 260/280 | 054426 |
| 0.25 | 0.25 | 30 | 20 to 260/280 | 054427 |
| 0.25 | 0.5 | 30 | 20 to 260/280 | 054415 |
| 0.25 | 1 | 30 | 30 to 240/260 | 054439 |
| 0.25 | 0.25 | 60 | 20 to 260/280 | 054428 |
| 0.25 | 0.5 | 60 | 20 to 260/280 | 054458 |
| 0.32 | 0.25 | 15 | 20 to 260/280 | 054432 |
| 0.32 | 0.25 | 25 | 20 to 260/280 | 054430 |
| 0.32 | 0.5 | 25 | 20 to 260/280 | 054436 |
| 0.32 | 1 | 25 | 20 to 240/260 | 054442 |
| 0.32 | 0.25 | 30 | 20 to 260/280 | 054433 |
| 0.32 | 0.5 | 30 | 20 to 260/280 | 054438 |
| 0.32 | 1 | 30 | 30 to 240/260 | 054444 |
| 0.32 | 0.25 | 50 | 20 to 260/280 | 054431 |
| 0.32 | 0.5 | 50 | 20 to 260/280 | 054437 |
| 0.32 | 1 | 50 | 20 to 240/260 | 054443 |
| 0.32 | 0.25 | 60 | 20 to 260/280 | 054434 |
| 0.32 | 0.5 | 60 | 20 to 260/280 | 054457 |
| 0.32 | 1 | 60 | 20 to 240/260 | 054445 |
| 0.53 | 1 | 12 | 20 to 240/260 | 054447 |
| 0.53 | 2 | 12 | 20 to 240/260 | 054455 |
| 0.53 | 0.5 | 15 | 20 to 260/280 | 054961 |
| 0.53 | 1 | 15 | 20 to 240/260 | 054450 |
| 0.53 | 1 | 25 | 20 to 240/260 | 054448 |
| 0.53 | 2 | 25 | 30 to 240/260 | 054456 |
| 0.53 | 0.5 | 30 | 20 to 260/280 | 054440 |
| 0.53 | 1 | 30 | 20 to 240/260 | 054451 |
| 0.53 | 0.5 | 60 | 20 to 260/280 | 054963 |
| 0.53 | 1 | 60 | 20 to 240/260 | 0544515 |

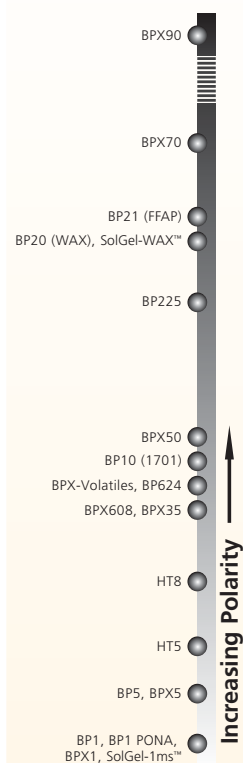


GC Columns and Applications




GC Capillary Columns | Polyethylene Glycol (PEG) – TPA Treated

BP21 (FFAP)

- Nitroterephthalic acid modified PEG.
- Polar phase.
- Ideal for low molecular weight acids.
- 240/250 °C upper temperature limit.
- Able to be solvent rinsed (water or methanol is NOT recommended for rinsing).
- Bonded and cross-linked.

| | |
|---|---|
| Especially Suitable for these Industries: |    |
| Application Areas: | Volatile free acids, fatty acid methyl esters, alcohols, aldehydes, acrylates, ketones. Applications AC102, SOL04. |
| Suitable Replacement for: | DB-FFAP, HP-FFAP, Stabilwax-DA, CPWax-58CB. |




GC Columns and Applications

BP21 (FFAP)




| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.22 | 0.25 | 25 | 35 to 240/250 | 054462 |
| 0.22 | 0.25 | 50 | 35 to 240/250 | 054463 |
| 0.25 | 0.25 | 15 | 35 to 240/250 | 054464 |
| 0.25 | 0.25 | 30 | 35 to 240/250 | 054465 |
| 0.25 | 0.25 | 60 | 35 to 240/250 | 054466 |
| 0.32 | 0.25 | 12 | 35 to 240/250 | 054467 |
| 0.32 | 0.25 | 15 | 35 to 240/250 | 054470 |
| 0.32 | 0.25 | 25 | 35 to 240/250 | 054468 |
| 0.32 | 0.25 | 30 | 35 to 240/250 | 054471 |
| 0.32 | 0.25 | 50 | 35 to 240/250 | 054469 |
| 0.32 | 0.25 | 60 | 35 to 240/250 | 054472 |
| 0.53 | 0.5 | 12 | 35 to 240/250 | 054473 |
| 0.53 | 0.5 | 15 | 35 to 240/250 | 054476 |
| 0.53 | 0.5 | 25 | 35 to 240/250 | 054474 |
| 0.53 | 0.5 | 30 | 35 to 240/250 | 054477 |
| 0.53 | 1 | 30 | 35 to 240/250 | 054478 |

GC Columns | 14% Cyanopropylphenyl Polysiloxane



BP10 (1701)

- Used for organochlorine pesticides analysis.
- Highly inert.
- Low bleed.
- 260/300 °C upper temperature limit - dependent on film thickness.
- Bonded and cross-linked.
- Able to be solvent rinsed.

| | |
|---|--|
| Especially Suitable for these Industries: |    Pharmaceuticals Environment Forensics |
| Application Areas: | Environmental analyses (EPA methods 608 and 8081), pesticides/herbicides, drugs of abuse, pharmaceuticals. |
| Suitable Replacement for: | DB-1701, Rtx-1701, SPB-7, HP-1701, CP-Sil 19CB, 007-1701, PE-1701, SP-1701. |

| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.22 | 0.25 | 12 | -20 to 280/300 | 054252 |
| 0.22 | 0.25 | 25 | -20 to 280/300 | 054253 |
| 0.22 | 0.25 | 50 | -20 to 280/300 | 054254 |
| 0.25 | 0.25 | 15 | -20 to 280/300 | 054255 |
| 0.25 | 0.25 | 30 | -20 to 280/300 | 054256 |
| 0.25 | 1 | 30 | -20 to 260/280 | 054271 |
| 0.25 | 0.25 | 60 | -20 to 280/300 | 054257 |
| 0.32 | 0.25 | 15 | -20 to 280/300 | 054258 |
| 0.32 | 0.5 | 15 | -20 to 280/300 | 054264 |
| 0.32 | 0.25 | 25 | -20 to 280/300 | 054262 |
| 0.32 | 0.5 | 25 | -20 to 280/300 | 054268 |
| 0.32 | 0.25 | 30 | -20 to 280/300 | 054259 |
| 0.32 | 0.5 | 30 | -20 to 280/300 | 054265 |
| 0.32 | 1 | 30 | -20 to 260/280 | 054270 |
| 0.32 | 0.5 | 50 | -20 to 280/300 | 054269 |
| 0.32 | 0.25 | 60 | -20 to 280/300 | 054260 |
| 0.32 | 0.5 | 60 | -20 to 280/300 | 054266 |
| 0.53 | 1 | 15 | -20 to 260/280 | 054282 |
| 0.53 | 1 | 25 | -20 to 260/280 | 054280 |
| 0.53 | 1 | 30 | -20 to 260/280 | 054283 |


Expert Tip :

Do not use plastic tubing in GC systems. Plastic tubing, when used for general plumbing, can absorb up to 20% moisture allowing external laboratory gases to permeate through the tubing. SGE recommends clean stainless steel tubing to be used throughout the GC system.





BP225

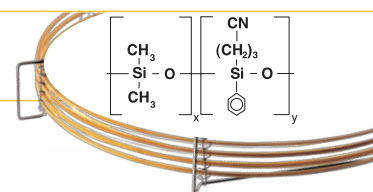- Mid to high polarity.
- Low bleed.
- Bonded and cross-linked.
- 230/260 °C upper temperature limit.
- Able to be solvent rinsed.



GC Columns and Applications


| | |
|---|---|
| Especially Suitable for these Industries: |   |
| Application Areas: | Fatty Acid Methyl Esters (FAMES), carbohydrates, neutral sterols. |
| Suitable Replacement for: | DB-225, HP-225 and RTX-225. |




| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.22 | 0.25 | 25 | 40 to 230/260 | 054352 |
| 0.22 | 0.25 | 50 | 40 to 230/260 | 054353 |
| 0.32 | 0.25 | 25 | 40 to 230/260 | 054358 |
| 0.53 | 0.5 | 25 | 40 to 230/260 | 054364 |

GC Columns | Cyanopropylphenyl Polysiloxane


BPX-VOLATILES

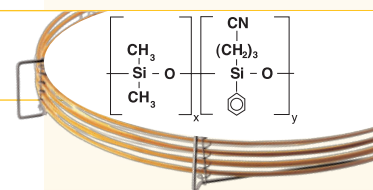- Polar phase.
- EPA volatile organics analysis (EPA 624, 502.2, SW-846 8240/8260).
- 290/300 °C upper temperature limit.
- Able to be solvent rinsed.
- Bonded and cross-linked.



| | |
|---|---|
| Especially Suitable for these Industries: |    |
| Application Areas: | Environmental analyses, volatile organics, alcohol analysis, USP G43. Application TP-0102-C. |
| Suitable Replacement for: | DB-VRX, HP-624, OPTIMA 624, ELITE-624, 007-624, RTX-VOLATILES, SPB-624, TRV1, CPSIL 13 CB, VOCOL, VB-624, CP-624. |


| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.18 | 1 | 20 | 0 to 290/300 | 054978 |
| 0.18 | 1 | 40 | 0 to 290/300 | 054979 |
| 0.25 | 1.4 | 30 | 0 to 290/300 | 054980 |
| 0.25 | 1.4 | 60 | 0 to 290/300 | 054981 |
| 0.32 | 1.8 | 30 | 0 to 290/300 | 054982 |
| 0.32 | 1.8 | 60 | 0 to 290/300 | 054983 |
| 0.53 | 3 | 30 | 0 to 290/300 | 054984 |
| 0.53 | 3 | 60 | 0 to 290/300 | 054985 |



BP624


GC Columns and Applications

- US EPA 624 optimized column.
- Designed for volatiles analysis.
- Ideal for EPA624, SW-846 methods 8240/8260.
- Ideal for USP G43 method.
- 230/240 °C upper temperature limit.
- Able to be solvent rinsed.
- Bonded and cross-linked.

| | |
|---|--|
| Especially Suitable for these Industries: |  Environment |
| Application Areas: | EPA method 624, drinking water volatiles, chlorinated hydrocarbons, solvents, Excellent for U.S. EPA Methods: 501.3, 502.2, 503.1, 524.2, 601, 602, 8010, 8015, 8020, 8240, 8260. Applications ENV17, ENV13. |
| Suitable Replacement for: | DB-624, OV-624, AT-624, HP-VOC, CP-Select624CB, 007-624, Rtx-Volatiles, Rtx 624, VOCOL, ZB-624. |



| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.22 | 1.2 | 25 | 0 to 230/240 | 054826 |
| 0.22 | 1.2 | 30 | 0 to 230/240 | 054827 |
| 0.25 | 1.4 | 15 | 0 to 230/240 | 054839 |
| 0.25 | 1.4 | 30 | 0 to 230/240 | 054840 |
| 0.25 | 1.4 | 60 | 0 to 230/240 | 054842 |
| 0.32 | 1.8 | 25 | 0 to 230/240 | 054830 |
| 0.32 | 1.8 | 30 | 0 to 230/240 | 054832 |
| 0.32 | 1.8 | 50 | 0 to 230/240 | 054831 |
| 0.32 | 1.8 | 60 | 0 to 230/240 | 054841 |
| 0.53 | 3 | 25 | 0 to 230/240 | 054834 |
| 0.53 | 3 | 30 | 0 to 230/240 | 054836 |
| 0.53 | 3 | 50 | 0 to 230/240 | 054835 |
| 0.53 | 3 | 60 | 0 to 230/240 | 054838 |

GC Columns | Permethyated Beta-Cyclodextrin (Chiral)



CYDEX-B™

- Separation of chiral compounds

| | |
|---|---|
| Especially Suitable for these Industries: |   Pharmaceuticals Food |
| Application Areas: | Separation of enantiomeric compounds found in natural products. Application FLA05. |
| Operating Temperature: | 30 °C to 220/240 °C |
| Suitable Replacement for: | Cyclodex-B, Rt-BDEXm, LIPODEX C |


| ID (mm) | Film Thickness (µm) | Length (m) | Temperature Limits (°C) | Part No. |
|---------|---------------------|------------|-------------------------|----------|
| 0.22 | 0.25 | 25 | 30 to 220/240 | 054900 |
| 0.22 | 0.25 | 50 | 30 to 220/240 | 054901 |
| 0.32 | 0.25 | 25 | 30 to 220/240 | 054902 |



GC Columns and Applications



ENV 62 | Polynuclear Aromatic Hydrocarbons (PAH) Analysis on BPX50

| | | | |
|--------------------------|------------------------------|------------------------------------|----------------------|
| Column Part No.: | 054751 | Flow: | On |
| Phase: | BPX50, 0.25 µm film | Average Linear Velocity: | 39 cm/sec at 65 °C |
| Column: | 30 m x 0.25 mm ID | Mode of Injection: | splitless |
| (PAH) standard: | 10 ng/ µL in dichloromethane | Purge on Time: | 0.5 min. |
| Initial Temp.: | 65 °C, 0.5 min | Purge on (split) Vent Flow: | 60 mL/min |
| Rate 1.: | 25 °C/min to 140 °C | Injection Volume: | 0.2 µL |
| Rate 2.: | 10 °C/min to 325 °C | Injection Temp.: | 250 °C |
| Final Temp.: | 325 °C, 15 min | Autosampler: | No |
| Detector Type: | MSD | Liner Type: | 4 mm ID Double Taper |
| Carrier Gas: | Helium, 9.7 psi | Liner Part Number: | 092018 |
| Carrier Gas Flow: | 1.1 mL/min constant | | |

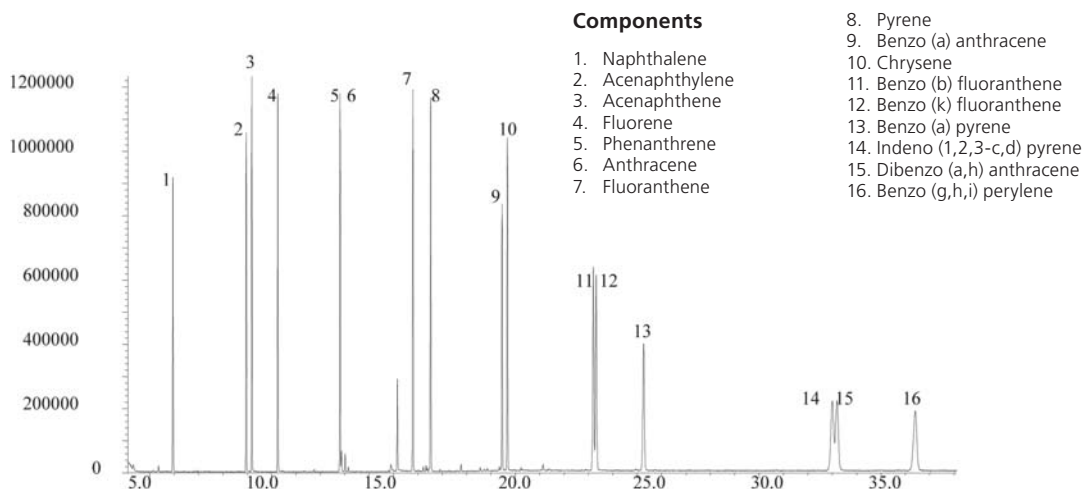

ARO 08 | Analysis of Polynuclear Aromatic Hydrocarbons on HT8

| | | | |
|-------------------------|-------------------|---------------------|---------------|
| Column Part No.: | 054462 | Rate: | 4 °C/min |
| Phase: | HT8, 0.25 µm film | Final Temp: | 380 °C, 5 min |
| Column: | 25 m x 0.22 mm ID | Carrier Gas: | He, 20 psi |
| Initial Temp: | 150 °C, 1 min | Detector: | FID |

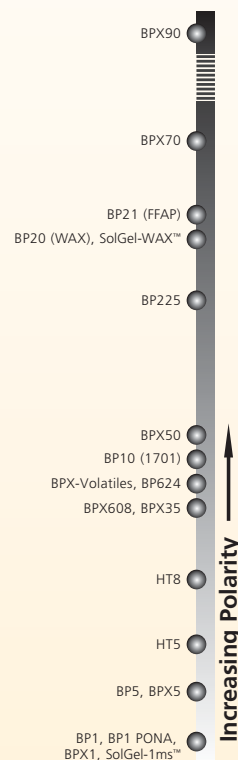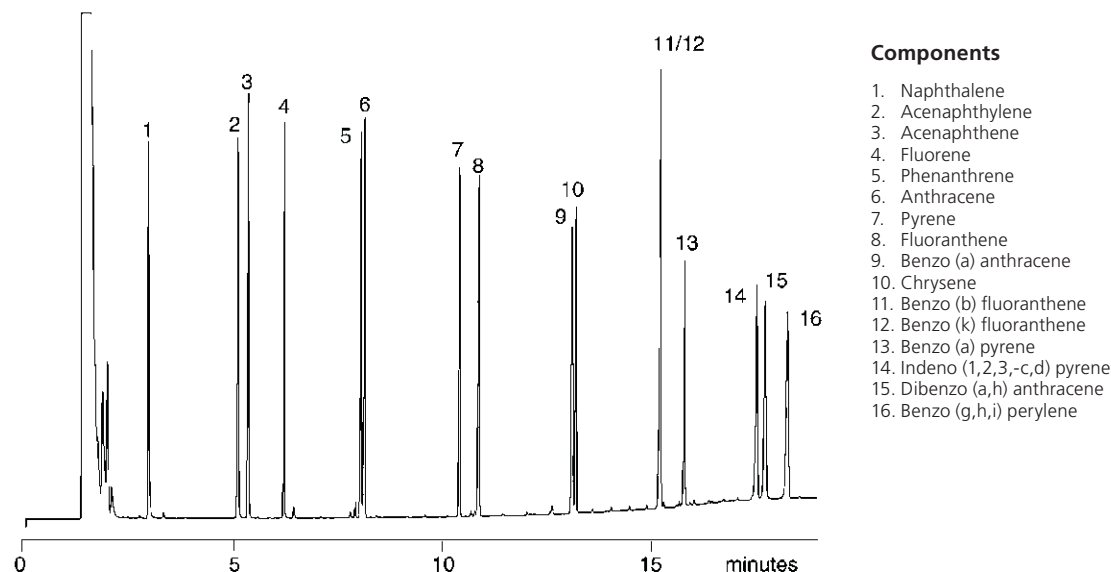





GC Columns and Applications

AP 0040C | HT8: The Perfect PCB Column

Separation of CB31 & CB28

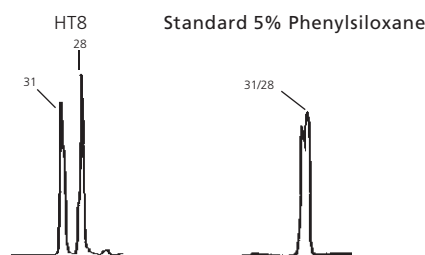

Chromatogram on the left clearly demonstrates the significant difference in selectivity of the HT8 column. By GC/MS, quantitation of CB28 using a standard 5% phenylpolysiloxane column is impossible as coelution with CB31 (with the same number of chlorines) occurs.

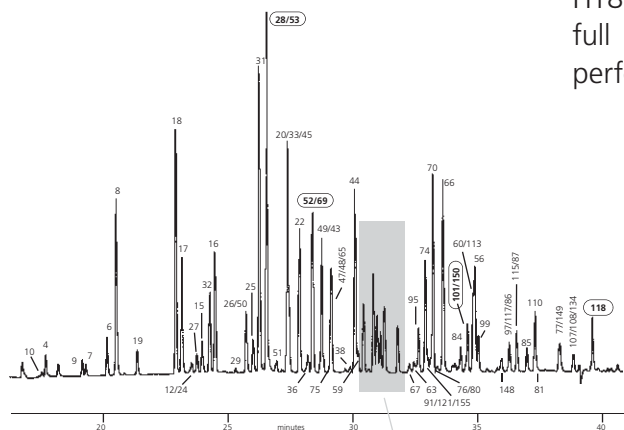

HT8 separates the two congeners by a full minute allowing quantitation to be performed with ease.

AROCLOR 1242

Column Part No.: 054676

Phase: HT8, 0.25 µm film

Column: 50 m x 0.22 mm ID

Initial Temp: 80 °C, 2 min

Rate 1: 30 °C/min

Temp 2: 170 °C


Rate 2: 3 °C/min

Final Temp: Split, 300 °C



Carrier Gas: He, 40 psi

Detector: ECD, 330 °C

| Congener # | Cl Position | Cl # | Identification by GC/MS |
|------------|-------------|------|-------------------------|
| 42 | 23-24 | 4 | ✓ |
| 96 | 236-26 | 5 | ✓ |
| 35 | 34-3 | 3 | ✓ |
| 64 | 235-4 | 4 | * |
| 72 | 25-35 | 4 | * |
| 103 | 246-25 | 5 | ✓ |
| 71 | 26-34 | 4 | ✓ |
| 41 | 234-2 | 4 | ✓ |
| 68 | 24-35 | 4 | ✓ |
| 37 | 34-4 | 3 | ✓ |
| 100 | 246-24 | 5 | ✓ |

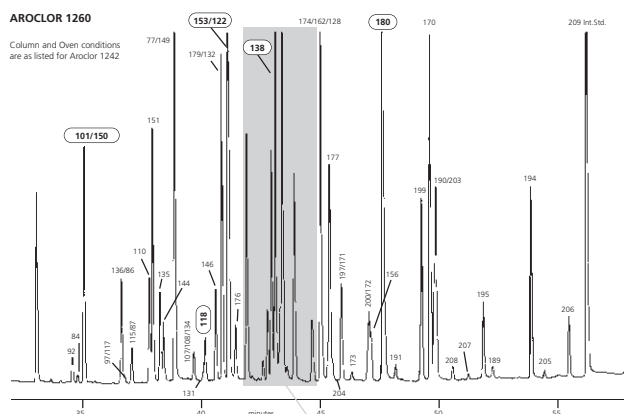

| Congener # | Cl Position | Cl # | Identification by GC/MS |
|------------|-------------|------|-------------------------|
| 42 | 23-24 | 4 | ✓ |
| 96 | 236-26 | 5 | ✓ |
| 35 | 34-3 | 3 | ✓ |
| 64 | 235-4 | 4 | * |
| 72 | 25-35 | 4 | * |
| 103 | 246-25 | 5 | ✓ |
| 71 | 26-34 | 4 | ✓ |
| 41 | 234-2 | 4 | ✓ |
| 68 | 24-35 | 4 | ✓ |
| 37 | 34-4 | 3 | ✓ |
| 100 | 246-24 | 5 | ✓ |

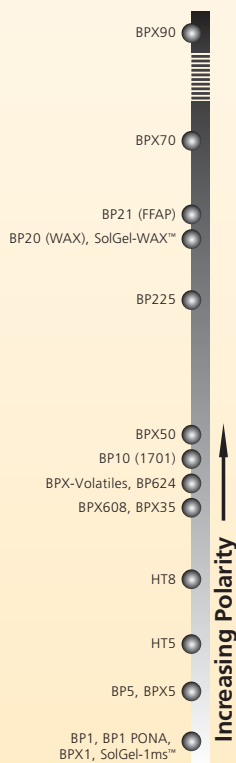


TP-0187-C | Analysis of Polynuclear Aromatic Hydrocarbons on BPX50

| | | | |
|-------------------------------|-----------------------------|-----------------------------|-------------------------------|
| Column Part No.: | 054701 | Temperature Profile: | Hold 70 °C for 1 min |
| Phase: | BPX50, 0.25 µm film | | 70 °C to 140 °C at 25 °C/min |
| Column: | 30 m x 25 µm ID | | 140 °C to 250 °C at 15 °C/min |
| Gas Flow: | 1.5 ml/min Helium | | 250 °C to 310 °C at 4 °C/min |
| Injection: | Split 1 µl (1 ng on column) | | Hold 310 °C for 8 min |
| Injection Temperature: | 250°C | | |




GC Columns and Applications

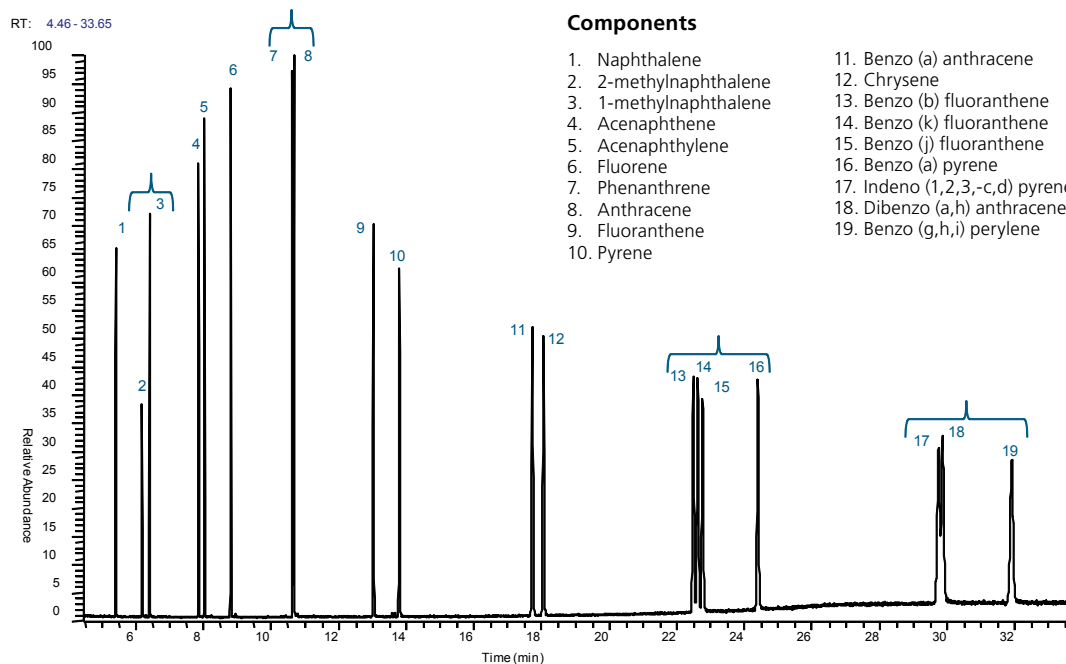

ENV 17 | Analysis of 16 Volatile Compounds in Drinking Water on BP624

| | | | |
|-------------------------|-------------------|------------------------|------------|
| Column Part No.: | 054826 | Final Temp.: | 170 °C |
| Phase: | BP624, 1.2 µm | Detector: | HP5870 MSD |
| Column: | 25 m x 0.22 mm ID | Injection Mode: | Splitless |
| Initial Temp.: | 50 °C, 2 min | Carrier Gas: | He, 15 psi |
| Rate: | 15 °C/min | | |

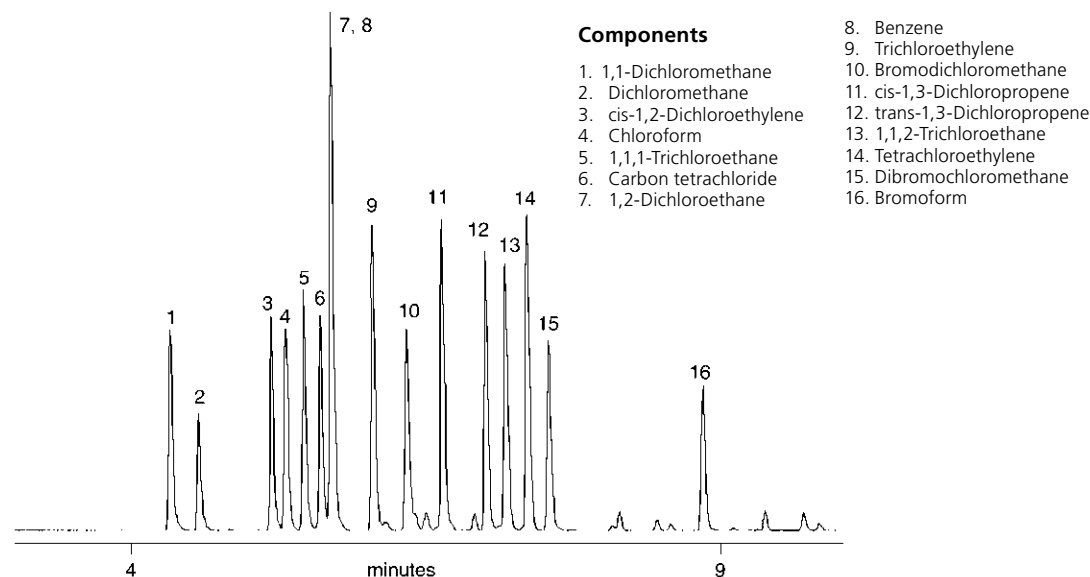





GC Columns and Applications

ENV 13 | Analysis of Volatiles from Drinking Water on BP624

| | | | |
|-------------------------|-------------------|-----------------|-------------------------|
| Column Part No.: | 054835 | | |
| Phase: | BP624, 3.0 µm | Rate 2: | 15 °C/min |
| Column: | 50 m x 0.53 mm ID | Final Temp.: | 210 °C, 1 min |
| Initial Temp.: | 35 °C, 2 min | Detector: | MSD, MJSC Jet Separator |
| Rate 1: | 8 °C/min | Injection Mode: | Purge & Trap |
| Temp 2: | 180 °C, 5 min | Carrier Gas: | He, 10 ml/min |

Note: Column which provides fast analysis of all EPA compounds. BP624 is also ideal for the analysis of many commonly used solvents.

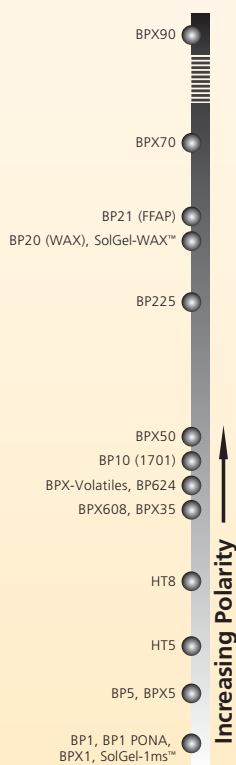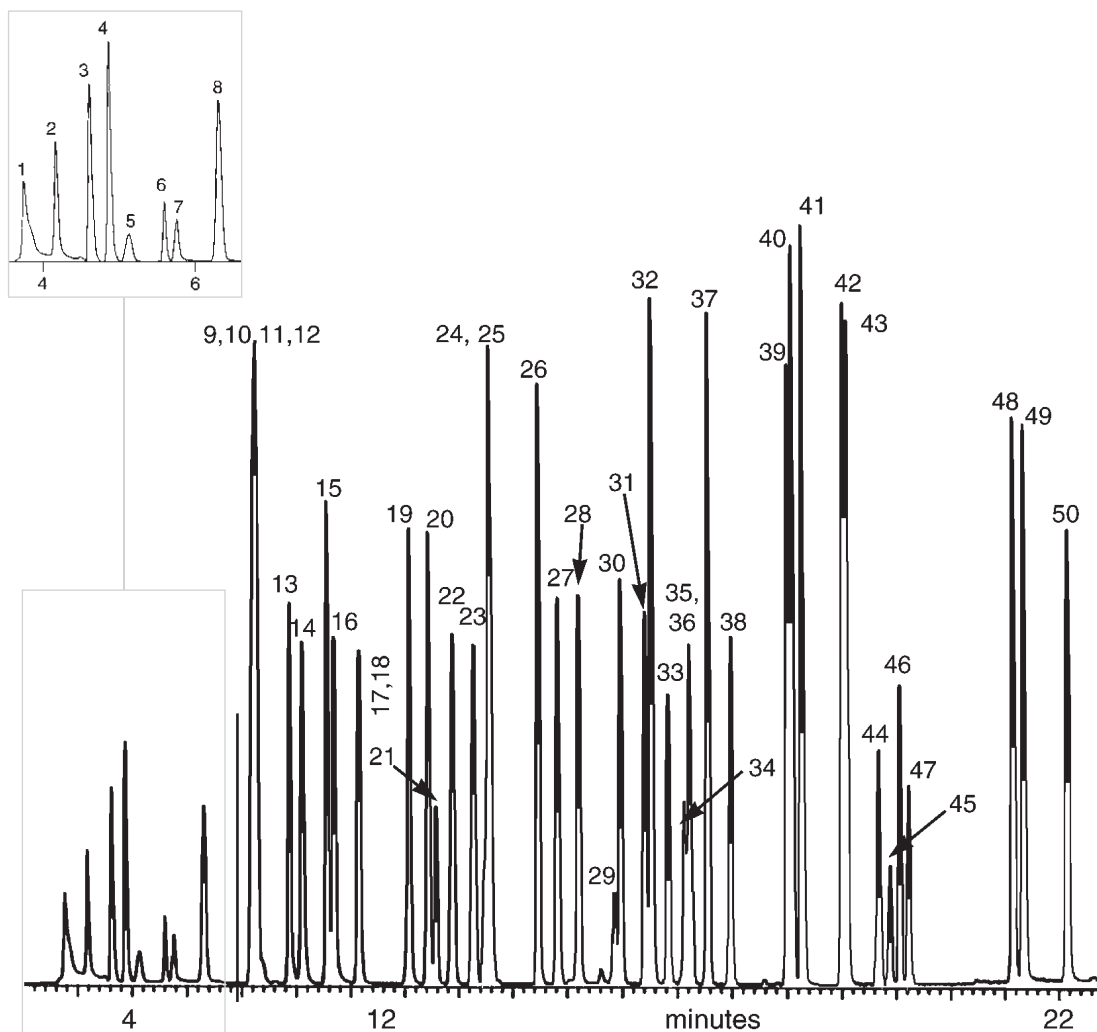

Components


- | | | |
|------------------------------|---------------------------------------|-----------------------------------|
| 1. Carbon dioxide | 17. 1,1-Dichloroethane | 35. 1,1,2-Trichloroethane |
| 2. Dichlorodifluoromethane | 18. Vinyl acetate | 36. 2-Hexanone |
| 3. Chloromethane | 19. 2-Butanone (MEK) | 37. Tetrachloroethene |
| 4. Vinyl chloride | 20. cis-1,2-Dichloroethene | 38. Dibromochloromethane |
| 5. Acetaldehyde | 21. Bromochloromethane (Int. Std.) | 39. Chlorobenzene |
| 6. Bromomethane | 22. 1,1,1-Trichloroethane | 40. Ethylbenzene |
| 7. Chloroethane | 23. Carbon tetrachloride | 41. m,p-Xylene |
| 8. Trichlorofluoromethane | 24. 1,2-Dichloroethane-d4 (Surrogate) | 42. o-Xylene |
| 9. Trichlorofluoroethane | 25. 1,2-Dichloroethane | 43. Styrene |
| 10. Acrolein | 26. Trichloroethene | 44. Bromoform |
| 11. Acetone | 27. 1,2-Dichloroethene | 45. 1,4-Dichlorobutane (Int. Std) |
| 12. 1,1-Dichloroethene | 28. Bromodichloromethane | 46. Bromofluorobenzene |
| 13. Carbon disulfide | 29. 4-Methyl-2-pentanone | 47. 1,1,2,2- Tetrachloroethene |
| 14. Methylene chloride | 30. cis-1,3-Dichloropropene | 48. 1,3-Dichlorobenzene |
| 15. trans-1,2-Dichloroethene | 31. Toluene-(d8) (Surrogate) | 49. 1,4-Dichlorobenzene |
| 16. Acrylonitrile | 32. Toluene | 50. 1,2-Dichlorobenzene |
| | 33. trans-1,3-Dichloropropene | |
| | 34. 2-Bromo-1-chloropropane (Int.Std) | |

TP-0102-C | Analysis of Volatile Organic Pollutants on a Volatiles GC Column



GC Columns and Applications

| | | | |
|-------------------|------------------------|--------------------------|----------------------|
| Column Part No.: | 054979 | Average Linear Velocity: | 35 cm/sec at 40 °C |
| Phase: | BPX-Volatiles 1µm film | Injection Mode: | Split |
| USEPA 502.2 mix: | 200 ppm in Methanol | Split Ratio: | 50:1 |
| Column: | 40m x 0.18mm ID | Injection Volume: | 1 µL |
| Initial Temp: | 40 °C, 0 min. | Injection Temperature: | 250 °C |
| Rate 1: | 6 °C to 210 °C | Autosampler: | No |
| Rate 2: | 15 °C to 250 °C | Liner Type: | 4 mm ID Single Taper |
| Final Temp: | 250 °C, 5 min | Liner Part Number: | 092017 |
| Detector Type: | Mass Spectrometer | Column Part Number: | 054979 |
| Carrier Gas: | He, 40.3 psi | ms-NoVent™ Part no.: | 113400 |
| Carrier Gas Flow: | 1.2 µL/min. | HP5973 restrictor: | 113409 |
| Constant Flow: | On | Full scan | 45-450 |

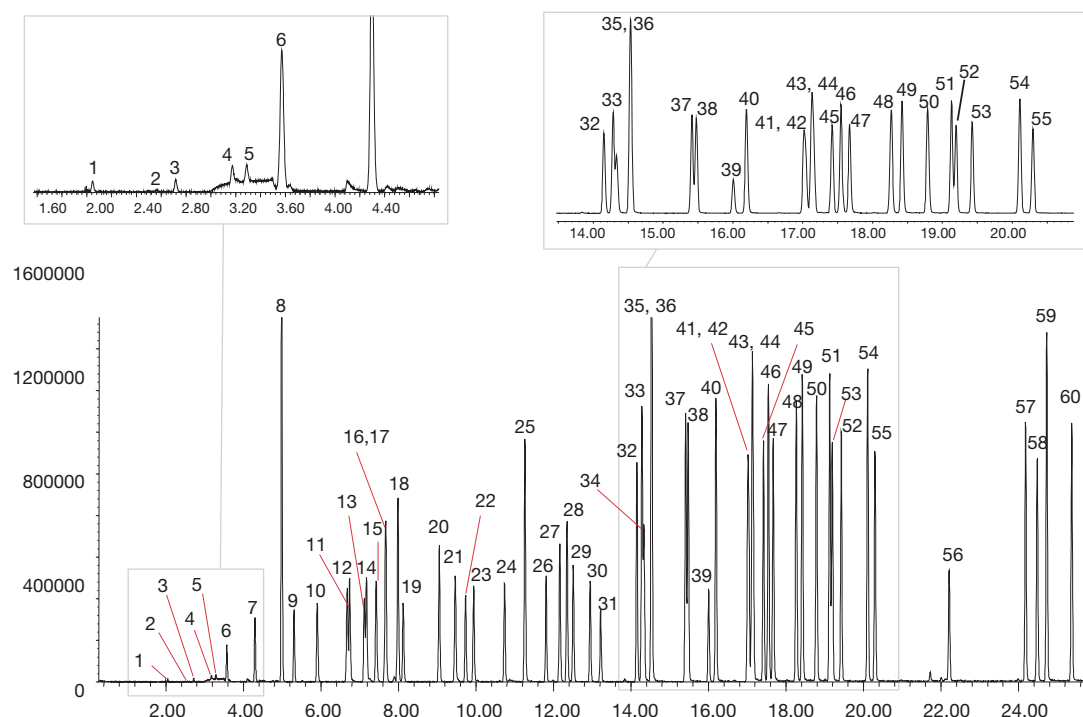

Notes. Chromatogram showing analysis of commonly screened volatile organic pollutants

Components

- | | | |
|-----------------------------|-------------------------------|---------------------------------|
| 1. Dichlorodifluoromethane | 20. Trichloroethene | 41. Bromobenzene |
| 2. Chloromethane | 21. 1,2-Dichloropropane | 42. 1,1,2,2-Tetrachloroethane |
| 3. Vinyl chloride | 22. Dibromomethane | 43. 1,2,3-Trichloropropane |
| 4. Bromomethane | 23. Bromodichloromethane | 44. n-Propyl benzene |
| 5. Chloroethane | 24. cis-1,3-Dichloropropene | 45. 2-Chlorotoluene |
| 6. Trichlorofluoromethane | 25. Toluene | 46. 1,3,5-Trimethylbenzene |
| 7. 1,1-Dichloroethene | 26. trans-1,3-Dichloropropene | 47. 4-Chlorotoluene |
| 8. Dichloromethane | 27. 1,1,2-Trichloroethane | 48. tert-Butylbenzene |
| 9. trans-1,2-Dichloroethene | 28. Tetrachloroethene | 49. 1,2,4-Trimethylbenzene |
| 10. 1,1-Dichloroethane | 29. 1,3-Dichloropropane | 50. sec-Butylbenzene |
| 11. 2,2-Dichloropropane | 30. Dibromochloromethane | 51. 1,3-Dichlorobenzene |
| 12. cis-1,2-Dichloroethene | 31. 1,2-Dibromoethane | 52. p-Isopropyltoluene |
| 13. Bromochloromethane | 32. Chlorobenzene | 53. 1,2-Dichlorobenzene |
| 14. Chloroform | 33. Ethylbenzene | 54. n-Butylbenzene |
| 15. 1,1,1-Trichloroethane | 34. 1,1,1,2-Tetrachloroethane | 55. 1,4-Dichlorobenzene |
| 16. 1,1-Dichloropropene | 35. p-Xylene | 56. 1,2-Dibromo-3-chloropropane |
| 17. Carbon tetrachloride | 36. m-Xylene | 57. 1,2,4-Trichlorobenzene |
| 18. Benzene | 37. o-Xylene | 58. Hexachlorobutadiene |
| 19. 1,2-Dichloroethane | 38. Styrene | 59. Naphthalene |
| | 39. Bromoform | 60. 1,2,3-Trichlorobenzene |
| | 40. Isopropylbenzene | |






GC Columns and Applications

ENV 20 | Analysis of Polychlorinated p-Dibenzodioxins on BPX5


| | |
|------------------|------------------------|
| Column Part No.: | 054114 |
| Phase: | BPX5, 0.25 μ m |
| Column: | 50 m x 0.22 mm ID |
| Initial Temp.: | 80 $^{\circ}$ C, 2 min |
| Rate 1: | 4 $^{\circ}$ C/min |
| Temp 2: | 220 $^{\circ}$ C |
| Rate 2: | 5 $^{\circ}$ C/min |

| | |
|-------------------|-----------------------------|
| Temp. 3: | 235 $^{\circ}$ C, 7 min |
| Rate 3: | 5 $^{\circ}$ C/min |
| Final Temp.: | 330 $^{\circ}$ C, 6 min |
| Detector: | High Resolution |
| Mass Spectrometer | He, 15 psi |
| Carrier Gas: | He, 300 psi |
| Injection Mode | Splitless, 270 $^{\circ}$ C |


Hexachlorodibenzodioxins

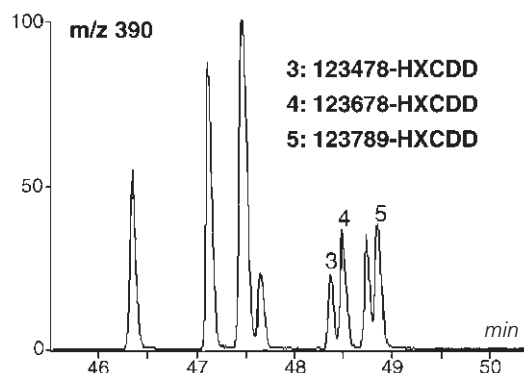


Tetrachlorodibenzodioxins

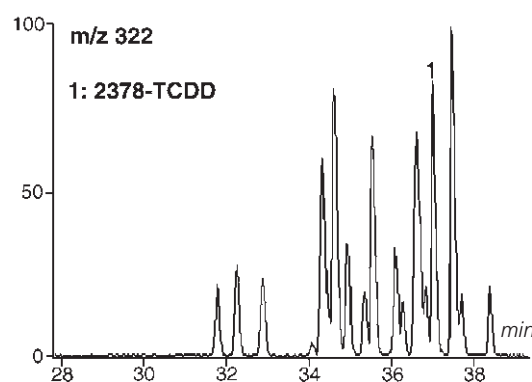


Heptachlorodibenzodioxins

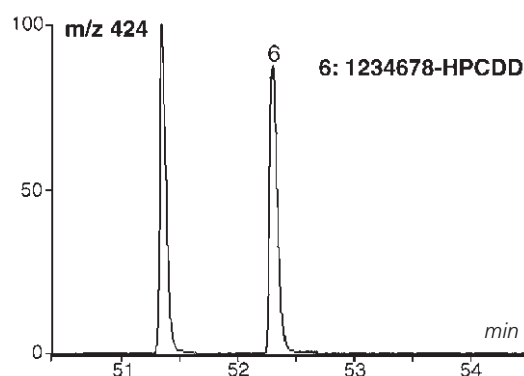


Pentachlorodibenzodioxins

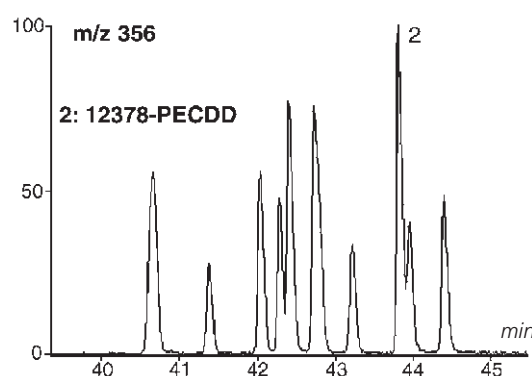

Octachlorodibenzodioxin

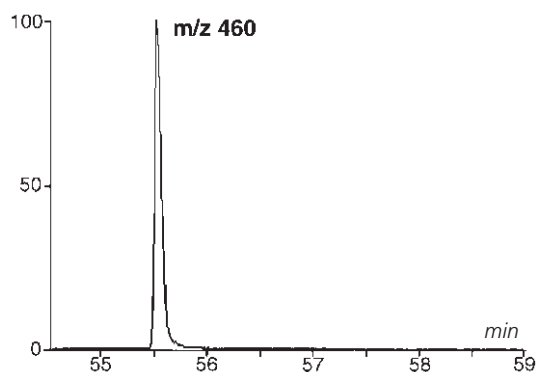

SGE wishes to acknowledge CARSO, 321 Avenue Jean Jaures, 69362 LYON CEDEX 7, FRANCE

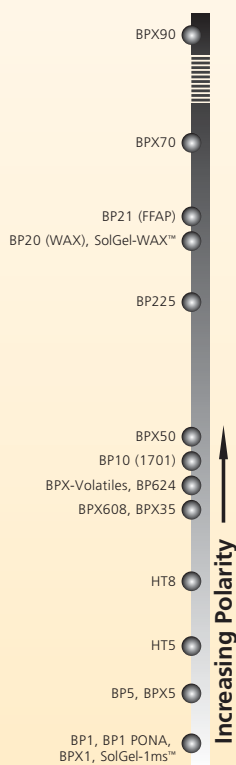


ENV 57 | 8081 Organochlorine Pesticide Mix on BPX35

| | | | |
|-------------------------|------------------------------|-----------------------------|----------------------------|
| Column Part No.: | 054701 | | |
| Phase: | BPX35 0.25 µm film | Constant Flow: | On |
| Column: | 30 m x 0.25 mm ID | Average Linear Velocity: | 36 cm/sec at 40 °C |
| 8081 Standard: | 10 ng/ µL in dichloromethane | Injection Mode: | Splitless |
| Initial Temp.: | 40 °C, 1 min. | Purge on Time: | 1 min. |
| Rate 1: | 30 °C to 190 °C, 3 min | Purge on (Split) Vent Flow: | 60 mL/min. |
| Rate 2: | 10 °C to 300 °C | Injection Volume: | 1 µL |
| Final Temp.: | 300 °C, 5 min. | Injection Temp.: | 250 °C |
| Detector Type: | MSD | Autosampler: | No |
| Carrier Gas: | He, 10.0 psi | Liner Type: | 4 mm ID Double Taper Liner |
| Carrier Gas Flow: | 1.3 mL/min | Liner Part Number: | 092018 |



GC Columns and Applications

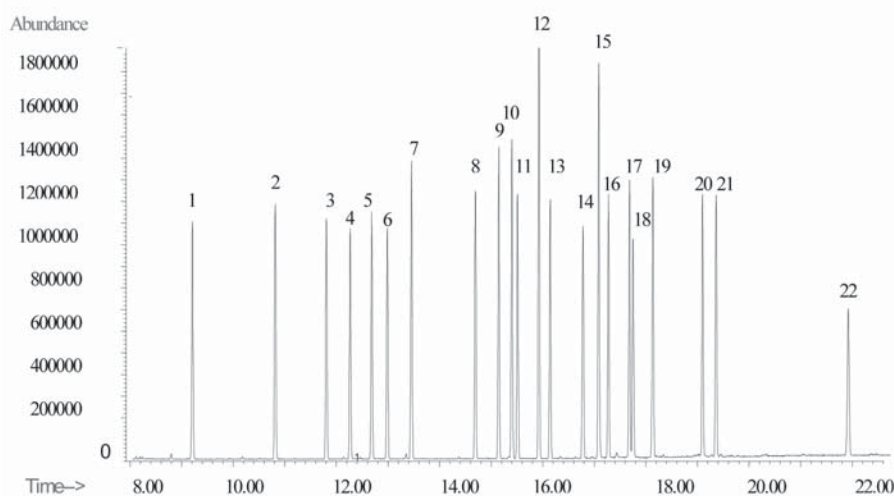

Components

1. 2,4,5,6-tetrachloro-meta-xylene
2. α-BHC
3. γ-BHC
4. β-BHC
5. Heptachlor
6. δ-BHC
7. Aldrin
8. Heptachlorepoxy
9. trans-Chlordane
10. cis-Chlordane
11. Endosulfan A
12. DDE
13. Dieldrin
14. Endrin
15. DDD
16. Endosulfan B
17. DDT
18. Endrin Aldehyde
19. Endosulfan Sulfate
20. Methoxychlor
21. Endrin Ketone
22. Decachlorobiphenyl

ENV 03 | Analysis of 18 Chlorinated Pesticides on BPX5


| | | | |
|------------------|-------------------|-----------------|---------------|
| Part No.: | 054125 | | |
| Phase: | BPX5, 0.5 µm film | Final Temp.: | 290 °C, 5 min |
| Column: | 25 m x 0.32 mm ID | Detector: | ECD at 310 °C |
| Initial Temp.: | 170 °C | Injection Mode: | Split |
| Rate: | 7 °C | Carrier Gas: | He, 7 psi |

Notes: Combined with the BPX608 column, BPX5 is the perfect confirmation column.

Components

20ng/ µL each component

1. α-BHC
2. γ-BHC
3. β-BHC
4. Heptachlor
5. δ-BHC
6. Aldrin
7. Heptachlorepoxy (isomer B)
8. Endosulfan I
9. 4,4'-DDE
10. Dieldrin
11. Endrin
12. 4,4'-DDD
13. Endosulfan II
14. 4,4'-DDT
15. Endrin aldehyde
16. Endosulfan sulfate
17. Methoxychlor
18. Endrin ketone

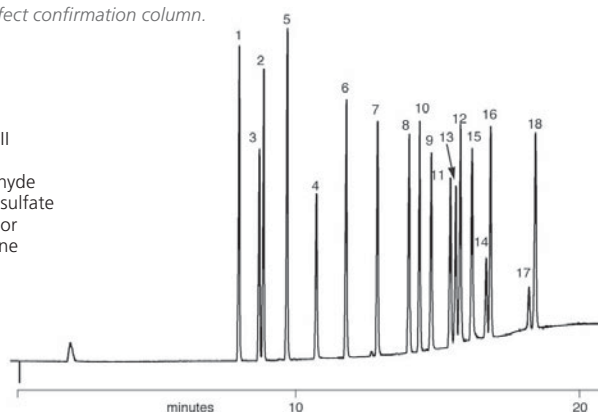





GC Columns and Applications

ENV 59 | 8141 Organophosphorous Pesticide Mix on BPX5

| | |
|-------------------------|------------------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| 8141 Standard: | 10 ng/ µL in dichloromethane |
| Initial Temp.: | 50 °C, 1 min |
| Rate 1: | 30 °C/min to 190 °C, 3 min |
| Rate 2: | 10 °C/min to 300 °C |
| Final Temp.: | 300 °C, 5 min. |
| Detector Type: | MSD |
| Carrier Gas: | He, 11.1 psi |
| Carrier Gas Flow: | 1.3 mL/min |

| | |
|-----------------------------|----------------------------|
| Constant Flow: | On |
| Average Linear Velocity: | 42 cm/sec at 50 °C |
| Injection Mode: | Splitless |
| Purge on Time: | 0.5 min |
| Purge on (Split) Vent Flow: | 60 mL/min |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Autosampler: | No |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

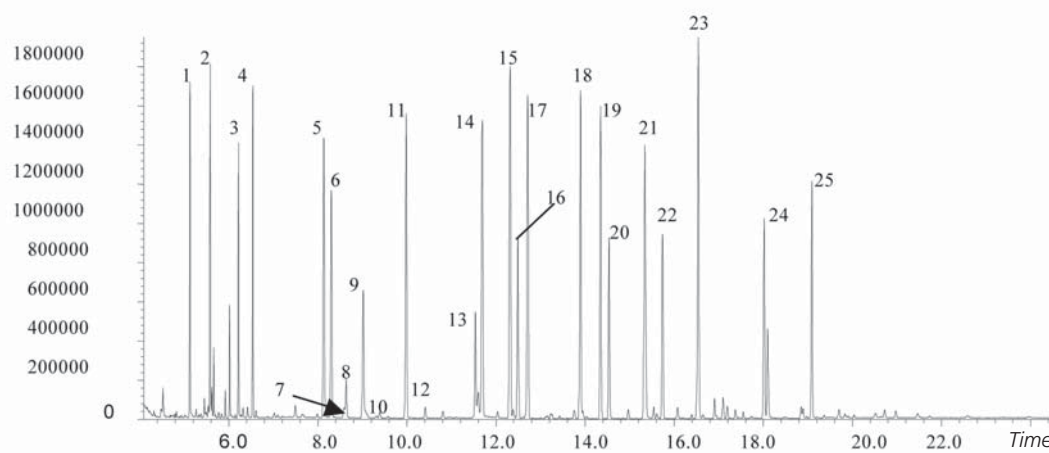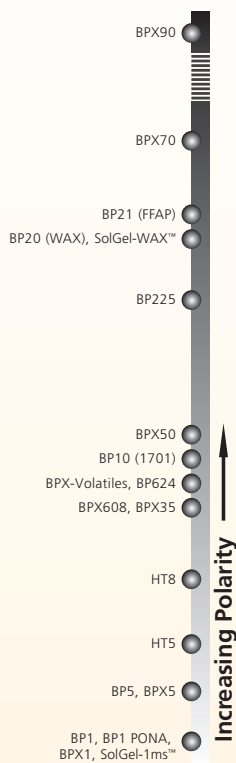

Components

- 4-Chloro-3-nitrobenzotrifluoride
- Dichlorvos
- 1-Bromo-2-nitrobenzene
- α-Mevinphos
- Tri-butylphosphate
- Ethoprop
- Sulfotepp

- Naled
- Phorate
- Demeton
- Diazinon
- Disulfoton
- Methyl parathion
- Ronnel
- Chlorpyrifos
- Fenthion

- Trichlorinate
- Tetrachlorvinphos
- Tokuthion
- Impurity
- Fensulfothion
- Impurity
- Triphenylphosphate
- Guthion
- Coumaphos

ENV 45 | Organophosphorous Pesticides on BPX50

| | |
|-------------------------------|---------------------------------------|
| Column Part No.: | 054751 |
| Phase: | BPX50, 0.25 µm film |
| Mixture of: | 10 ng/ µL |
| Organophosphorous Pesticides: | 10 ng/ µL in |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp: | 50 °C , 1 min |
| Rate 1: | 30 °C/min to 200 °C, 3 min |
| Rate 2: | 10 °C/min to 310 °C |
| Final Temp: | 310 °C, 2 min |
| Detector Type: | FID, 320 °C |
| Carrier Gas: | He, 14.4 psi |
| Carrier Gas Flow: | 1.30 mL/min |
| Constant Flow: | On |
| Average Linear Velocity: | 30 cm/sec at 50 °C |
| Injection Mode: | Splitless |
| Purge On Time: | 0.5 min |
| Purge On (Split) Vent Flow: | 60 mL/min |
| Injection Volume: | 1.0 µL |
| Injection Temperature: | 240 °C |
| Autosampler: | Yes |
| Liner Type: | 4 mm ID FocusLiner™ with single taper |
| Liner Part Number: | 092003 |


| | |
|------------------------------|-----------------------|
| Column Part Number: | 054740 |
| Phase: | BPX50, 0.10 µm film |
| Mixture of 10 ng/ µL | 42 cm/sec at 50 °C |
| Organophosphorous Pesticides | Splitless |
| Column: | 10 m x 0.10 mm ID |
| Initial Temp.: | 70 °C , 1 min |
| Rate 1: | 25 °C/min to 320 °C |
| Rate 2: | N/A |
| Final Temp: | 320 °C, 0 min |
| Detector Type: | FID, 320 °C |
| Carrier Gas: | He, 39.0 psi |
| Carrier Gas Flow : | 0.370 mL/min |
| Constant Flow: | On |
| Average Linear Velocity: | 35 cm/sec at 70 °C |
| Injection Mode: | Split |
| Purge On Time: | 1.0 |
| Purge On (Split) Vent Flow: | 10 mL/min |
| Injection Volume: | 0.5 µL |
| Injection Temperature: | 240 °C |
| Autosampler: | Yes |
| Liner Type : | 2.3 mm ID FocusLiner™ |
| Liner Part Number: | 092005 |



GC Columns and Applications

NORMAL

Chromatogram showing separation of Organophosphorous Pesticides using a conventional 30 meter x 0.25 mm ID BPX50 column with a 0.25 micron film.

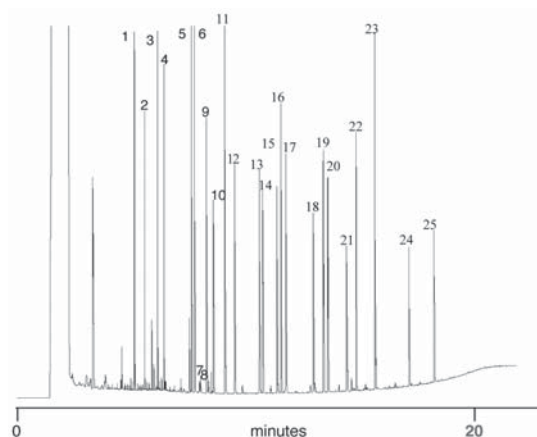


Components

- | | |
|--------------------------------------|----------------------|
| 1. 4-Chloro-3-nitrobenzo-trifluoride | 8. Naled |
| 2. Dichlorvos | 9. Phorate |
| 3. 1-Bromo-2-nitrobenzene | 10. Demeton |
| 4. α-Mevinphos | 11. Diazinon |
| 5. Tributylphosphate (IS) | 12. Disulfoton |
| 6. Ethoprop | 13. Methyl Parathion |
| 7. Sulfotepp | 14. Ronnel |
| | 15. Chlorpyrifos |
| | 16. Fenthion |

FAST

Chromatogram showing separation of Organophosphorous Pesticides using a FAST BPX50 column.

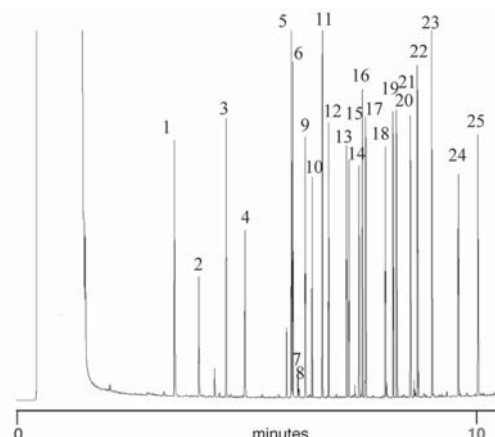

- | |
|-----------------------------|
| 17. Trichlorinate |
| 18. Tetrachlorvinphos |
| 19. Tokuthion |
| 20. Impurity |
| 21. Fensulfothion |
| 22. Impurity |
| 23. Triphenylphosphate (IS) |
| 24. Guthion |
| 25. Coumaphos |





GC Columns and Applications

ENV 04 | Analysis of Herbicides on BPX35

Column Part No.: 054711

Phase: BPX35, 0.25 µm film

Column: 25 m x 0.22 mm ID

Initial Temp.: 80 °C

Rate: 10 °C/min


Final Temp.: 300 °C 5 min

Detector: FID, 380 °C

Injection Mode: Split (20:1)

Carrier Gas: He, 100 kpa

Note: BPX35 provides quick analysis of all 3 Triazine compounds

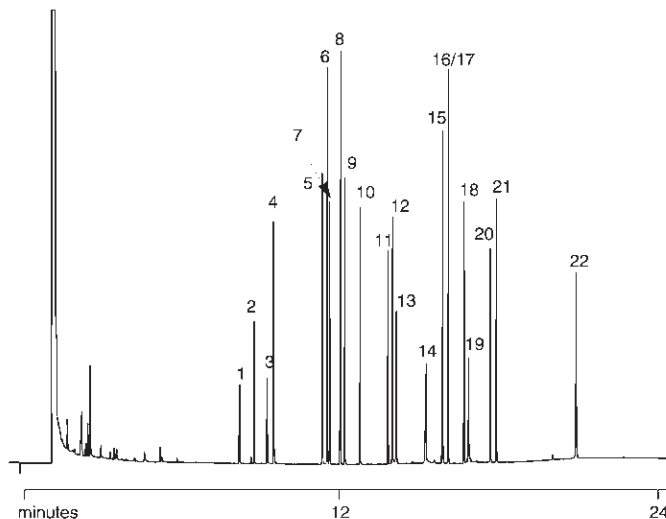

Components

1. Eptam®
2. Sutan®
3. Vernam®
4. Tillam®
5. Ordram®
6. Treflan®
7. Balan®
8. Ro-Neet®
9. Propachlor
10. Tolban®
11. Propazine
12. Atrazine
13. Simazine
14. Terbacil
15. Sencor®
16. Dual®
17. Paarlan®
18. Prowl®
19. Bromacil
20. Oxadiazon
21. GOAL®
22. Hexazinone

ENV 48 | Analysis of Herbicides on BPX5

Column Part No.: 054101

Phase: BPX5, 0.25 µm

Column: 30 m x 0.25 mm ID

Initial Temp.: 90 °C, 1 min

Rate 1: 30 °C/min

Temp.: 180 °C


Rate 2: 5 °C/min

Final Temp.: 260 °C, 10 min

Detector: NPD


Injection Mode: Varian SPI

Carrier Gas: He, 10 psi

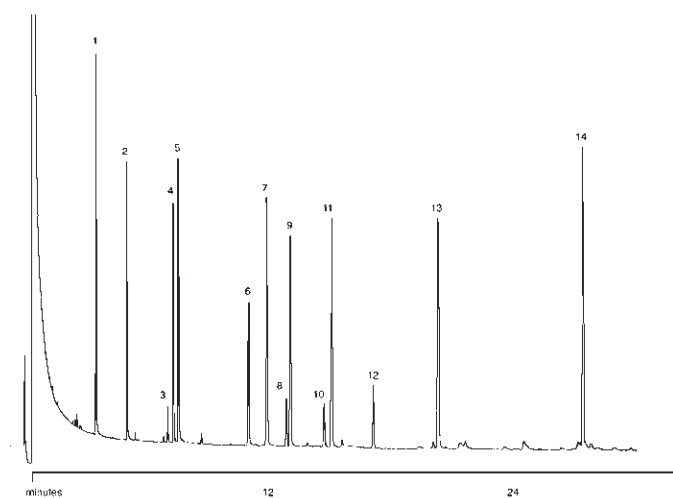

Components

1. Metamidofos
2. Acephate
3. Diphenylamine
4. Monocrofos
5. Sulfotep
6. Tolclofos-methyl
7. Fenitrothion
8. Triadimefon
9. Trichloronate
10. Triadimenol
11. Bromophos-ethyl
12. Bupirimate
13. Carbophenothion
14. Dialifos

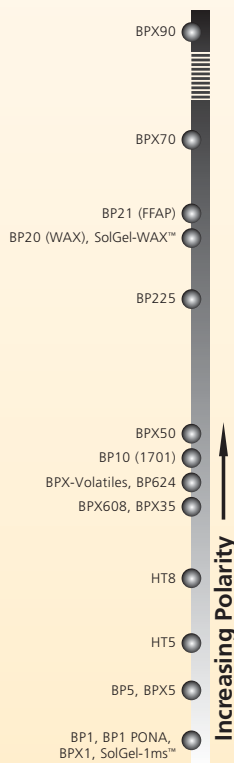




GC Columns and Applications

ARO 14 | Analysis of chlorinated and nitroaromatic compounds on SolGel-1ms™

| | | | |
|-------------------------|----------------------------|--------------------------|----------------------------|
| Column Part No.: | 054462 | Constant Flow: | On |
| Phase: | SolGel-1ms™ 0.25 µm film | Average Linear Velocity: | 35 cm/sec, 40 °C |
| Sample: | 200 ppm in dichloromethane | Injection Mode: | Split |
| Column: | 30 m x 0.25 mm ID | Split Ratio: | 100 : 1 |
| Initial Temp: | 40 °C, 1 min. | Injection Volume: | 0.5 µL |
| Rate 1: | 10 °C/min to 300 °C | Injection Tem: | 250 °C |
| Final Temp: | 300 °C, 2 min. | Liner Type: | 4 mm ID Single Taper Liner |
| Detector Type: | MSD | Liner Part No.: | 092017 |
| Carrier Gas: | He, 25.7 psi | Full Scan / SIM: | Full scan 45-450 |
| Carrier Gas Flow: | 1.8 mL/min. | | |

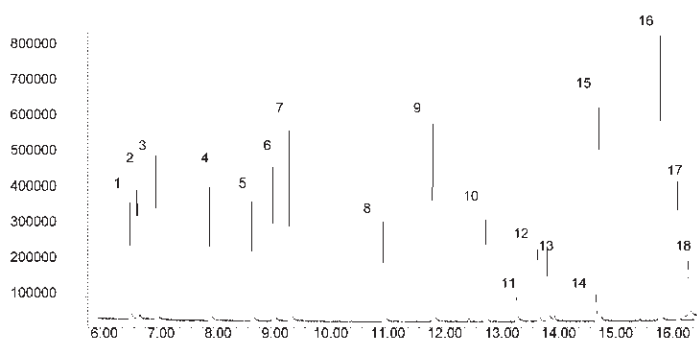


Components

1. Phenol
2. o-Chlorophenol
3. p-Dichlorobenzene
4. Nitrobenzene
5. o-Nitrophenol
6. 2,4-Xylenol
7. 2,4-Dichlorophenol
8. 4-Chloro-3-methylphenol
9. 2,4,6-Trichlorophenol
10. 2,6-Dinitrotoluene
11. 2,4-Dinitrophenol
12. 2,4-Dinitrotoluene
13. 4-Nitrophenol
14. 4,6-Dinitro-o-cresol
15. 4-Chlorophenyl phenyl ether
16. 4-Bromophenyl phenyl ether
17. Hexachlorobenzene
18. Pentachlorophenol

ALC 06 | US EPA 625 Phenols Mix on BPX50

| | | | |
|-------------------------|-------------------|--------------------|----------------|
| Column Part No.: | 054751 | Initial Oven Temp: | 50 °C, 1 min |
| Phase: | BPX50, 0.25 µm | Rate 1: | 8 °C/min |
| Column: | 30 m x 0.25 mm ID | Final Temp: | 300 °C, 10 min |
| Injector Mode: | Split, 40:1 | Detector: | HP 5973 MSD |

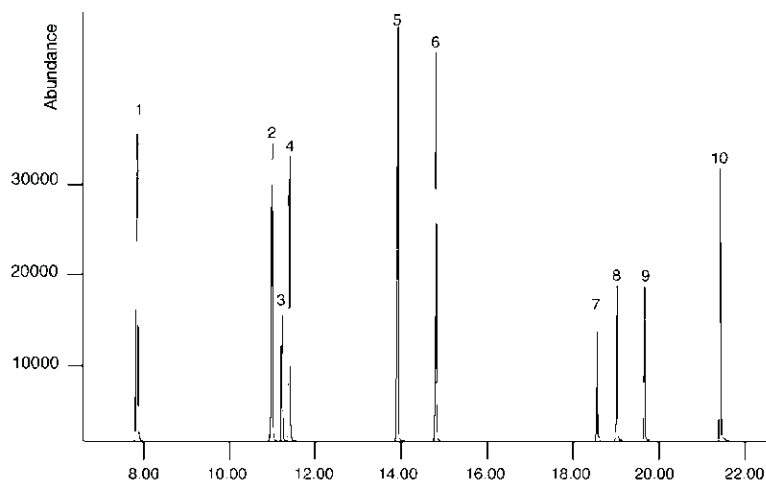

Components

1. 2-Chlorophenol
2. 2-Nitrophenol
3. 2, 4-Dimethylphenol
4. 2, 4-Dichlorophenol
5. 4-Chloro-3-methylphenol
6. 2, 4, 6-Trichlorophenol
7. 2, 4- Dinitrophenol
8. 4-Nitrophenol
9. 2-Methyl-4, 6-dinitrophenol
10. Pentachlorophenol






GC Columns and Applications



ENV 65 | Analysis of Synthetic Pyrethroids on BPX50

| | | | |
|-------------------------|----------------------|-----------------------------|----------------------------|
| Column Part No.: | 054751 | | |
| Phase: | BPX50, 0.25 µm film | Constant Flow: | On |
| Column: | 30 m x 0.25 mm ID 16 | Average Linear Velocity: | 36 cm/sec at 50 °C |
| Pyrethroids: | 10 ppm in methanol | Injection Mode: | Splitless |
| Initial Temp.: | 50 °C, 1 min. | Purge on Time: | 0.5 min |
| Rate 1: | 30 °C/min to 200 °C | Purge on (Split) Vent Flow: | 60 mL/min |
| Rate 2: | 4 °C/min to 300 °C | Injection Volume: | 1 µL |
| Final Temp.: | 300 °C, 5 min | Injection Temperature: | 250 °C |
| Detector Type: | MSD | Autosampler: | No |
| Carrier Gas: | He, 6.8 psi | Liner Type: | 4 mm ID Double Taper Liner |
| Carrier Gas Flow: | 1.0 mL/min | Liner Part Number: | 092018 |

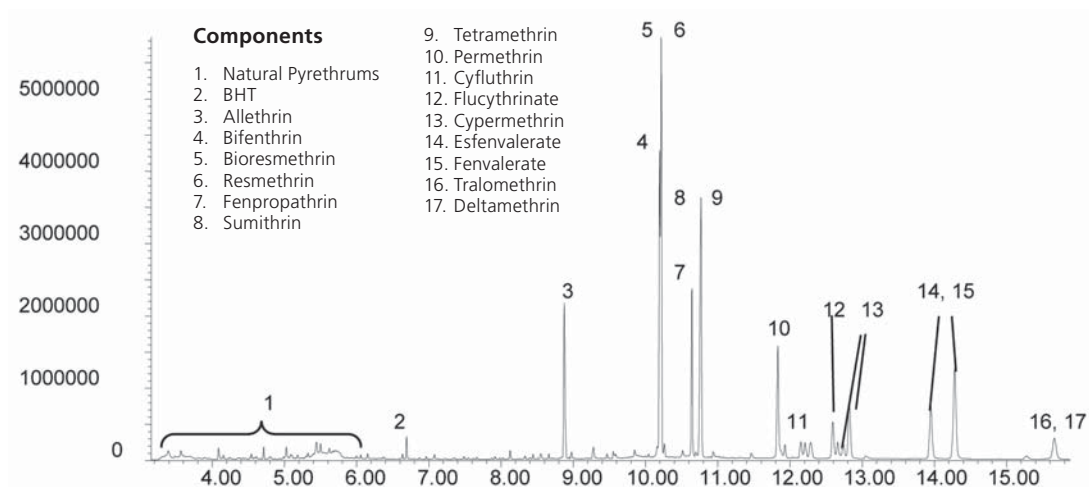

ARO 13 | Analysis of BTEX on SolGel-WAX™

| | | | |
|-------------------------|--------------------------|--------------------------|---------------------------|
| Column Part No.: | 054796 | | |
| Phase: | SolGel-WAX™ 0.25 µm film | Constant Flow: | On |
| BTEX: | 300 ppm in methanol | Average Linear Velocity: | 35 cm/sec, 60 °C |
| Column: | 30 m x 0.25 mm ID | Injection Mode: | Split |
| Initial Temp: | 60 °C, 10 min | Split Ratio: | 100:1 |
| Detector Type: | FID | Injection Volume: | 0.2 µL |
| Carrier Gas: | He, 17.3 psi | Injection Temp: | 250 °C |
| Carrier Gas Flow: | 1.5 mL/min | Liner Type: | 4 mm ID Double Taper Line |
| | | Liner Part Number: | 092018 |

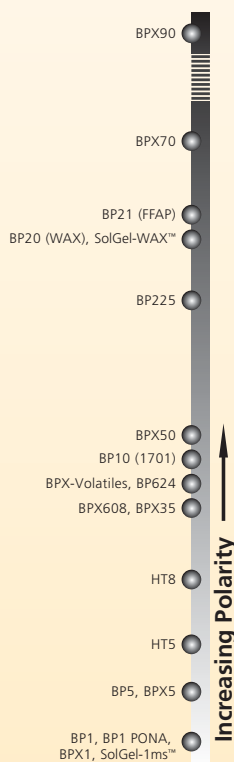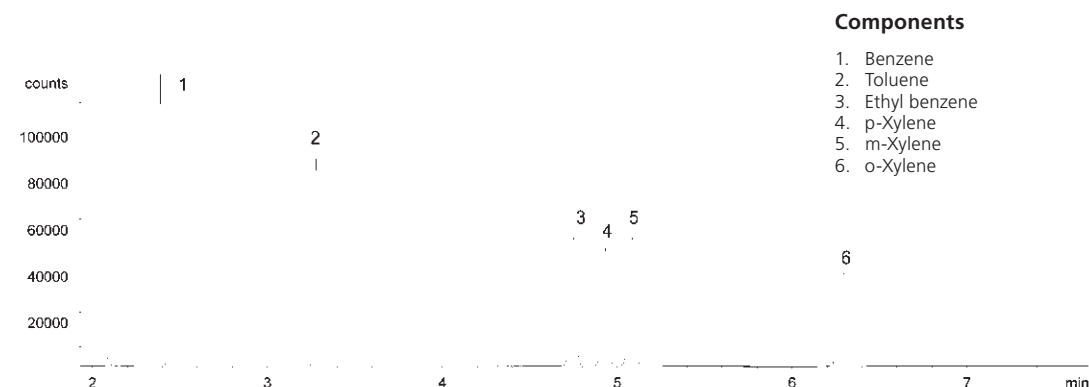


ENV 84 | Analysis of US EPA 8270 Mix on BPX5

| | | | |
|-------------------------|--|-----------------------------|--------------------------|
| Column Part No.: | 054101 | | |
| Phase: | BPX5, 0.25 µm film | Carrier Gas Flow: | 1.1 mL/min. |
| Column: | 30 m x 0.25 mm | Constant Flow: | On |
| ID Sample: | 5 ppm solution | Injection Mode: | Splitless |
| Initial Temp.: | 40 °C, 3 min | Purge on Time: | 0.5 min |
| Rate 1: | 8 °C/min to 300 °C | Purge on (Split) Vent Flow: | 40 mL/min |
| Final Temp.: | 300 °C, 9 min. | Injection Volume: | 1 µL |
| Detector Type: | Mass Spectrometer | Injection Temperature: | 250 °C |
| Carrier Gas: | He | Autosampler: | No |
| Inlet Pressure: | 16 psi for 30 sec then drops to 10 psi | Liner Type: | 4 mm ID Single Gooseneck |
| Pressure rate1: | 10 psi to 28 psi at 0.5 psi/min | Liner Part Number: | 092017 |
| Final Pressure: | 28 psi until end of run | Full Scan / SIM: | Full scan 41-450 |



GC Columns and Applications

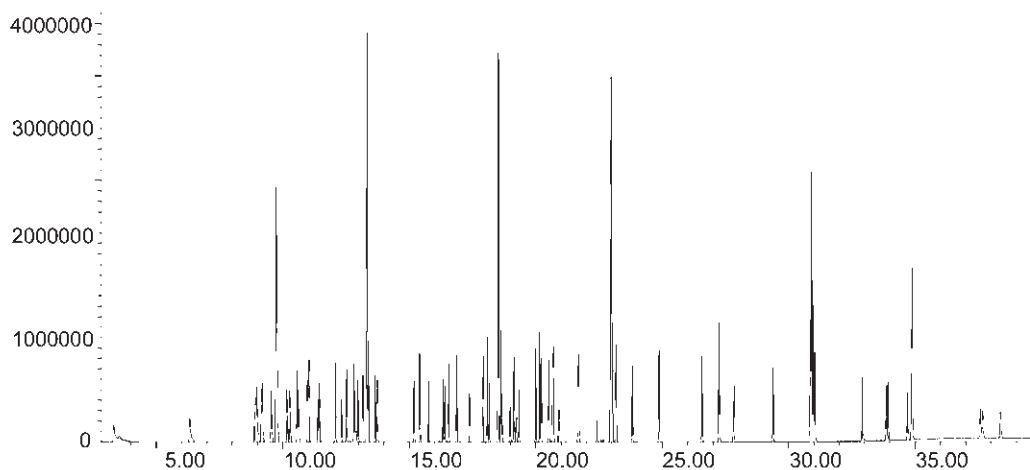

Components





- | | | |
|-----------------------------------|---------------------------------|----------------------------------|
| 1. Pyridine | 28. Naphthalene-d8 | 57. 2,4,6-Tribromophenol |
| 2. n-Nitrosodimethylamine | 29. Naphthalene | 58. 4-Bromophenyl phenyl ether |
| 3. 2-Fluorophenol | 30. Hexachlorobutadiene | 59. Hexachlorobenzene |
| 4. Phenol-d5 | 31. 4-Chloroaniline | 60. Pentachlorophenol |
| 5. Phenol | 32. 4-Chloro-3-methylphenol | 61. Phenanthrene-d10 |
| 6. Aniline | 33. 2-Methylnaphthalene | 62. Phenanthrene |
| 7. 2-Chlorophenol | 34. Hexachlorocyclopentadiene | 63. Anthracene |
| 8. bis- (2-chloroethyl) ether | 35. 2,4,6-Trichlorophenol | 64. Carbazole |
| 9. 1,3-Dichlorobenzene | 36. 2,4,5-Trichlorophenol | 65. Di-n-butyl phthalate |
| 10. 1,4-Dichlorobenzene-d4 | 37. 2-Fluorobiphenyl | 66. Fluoranthene |
| 11. 1,4-Dichlorobenzene | 38. 2-Chloronaphthalene | 67. Benzidine |
| 12. 1,2-Dichlorobenzene | 39. 2-Nitroaniline | 68. Pyrene |
| 13. Benzyl alcohol | 40. Dimethyl phthalate | 69. p-Terphenyl-d14 |
| 14. 2-Methyl phenol | 41. Acenaphthylene | 70. Butyl benzyl phthalate |
| 15. bis-(2-chloroisopropyl)ether | 42. 2,6-Dinitrotoluene | 71. Benz[a]anthracene |
| 16. n-Nitroso-di-n-propylamine | 43. Acenaphthene-d10 | 72. Chrysene-d12 |
| 17. Hexachloroethane | 44. Acenaphthene | 73. Chrysene |
| 18. 4-Methylphenol | 45. 3-Nitroaniline | 74. 3,3-Dichlorobenzidine |
| 19. Nitrobenzene-d5 | 46. 2,4-Dinitrophenol | 75. bis (2-Ethylhexyl) phthalate |
| 20. Nitrobenzene | 47. Dibenzofuran | 76. Di-n-octyl phthalate |
| 21. Isophorone | 48. 4-Nitrophenol | 77. Benzo (b) fluoranthene |
| 22. 2-Nitrophenol | 49. 2,4-Dinitrotoluene | 78. Benzo (k) fluoranthene |
| 23. 2,4-Xylenol | 50. Diethylphthalate | 79. Benzo (a) pyrene |
| 24. bis- (2-Chloroethoxy) methane | 51. Fluorene | 80. Perylene-d12 |
| 25. Benzoic acid | 52. 4-Chlorophenyl phenyl ether | 81. Indeno (1,2,3-cd) perylene |
| 26. 2,4-Dichlorophenol | 53. 2-Methyl-4,6-dinitrophenol | 82. Dibenz (a,h) anthracene |
| 27. 1,2,4-Trichlorobenzene | 54. 4-Nitroaniline | 83. Benzo[g,h,i]perylene |
| | 55. n-Nitrosodiphenylamine | |
| | 56. Azobenzene | |





GC Columns and Applications

ENV 84 continued

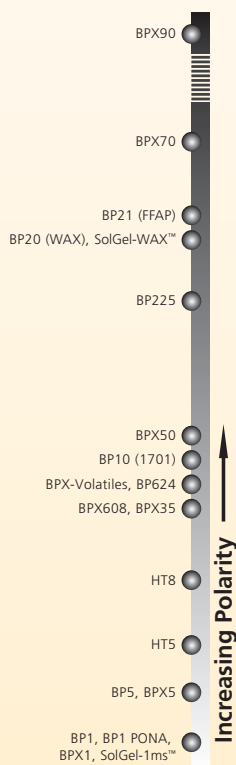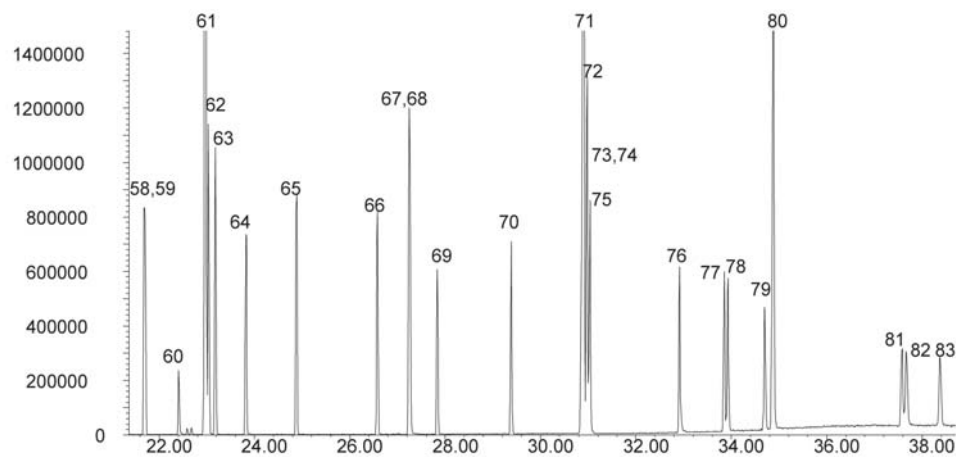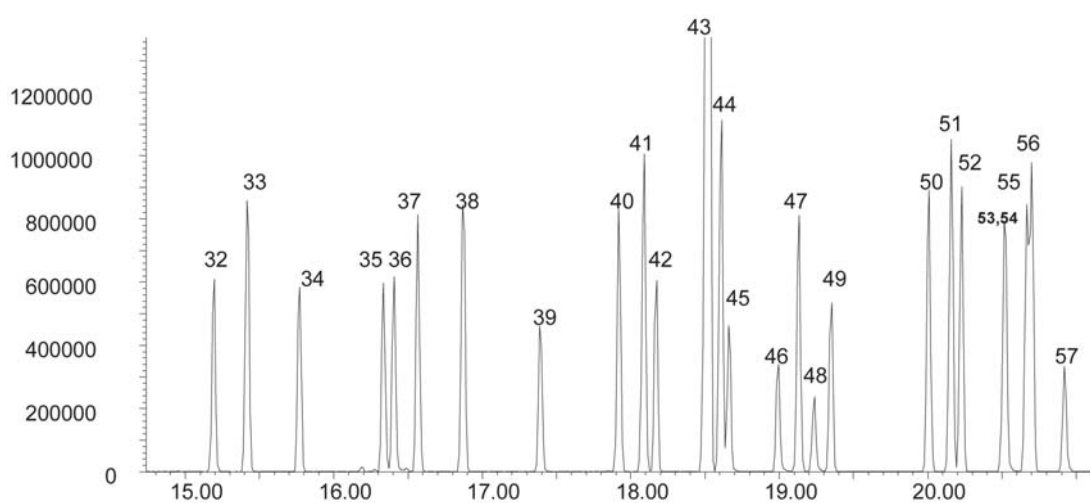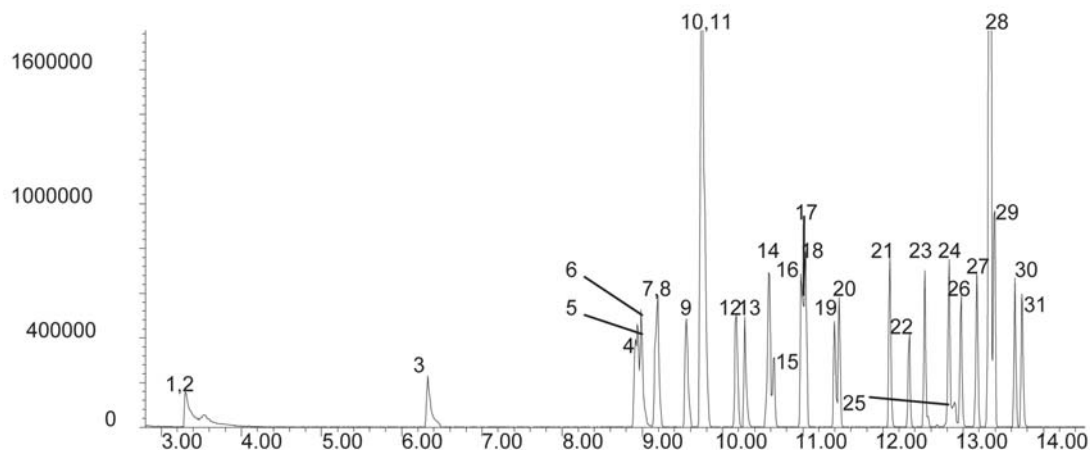


SGE would like to thank Mark Ferry from ECS/MDL USA for supplying all of the chromatograms for this application note.

FOO 03 | Analysis of Scotch Whisky on BP20

| | |
|-------------------------|-----------------------------|
| Column Part No.: | 054447 |
| Phase: | BP20, 1.0 µm film |
| Column: | 12 m x 0.53 mm ID |
| Initial Temp: | 55 °C, 3 min |
| Rate: | 10 °C/min |
| Final Temp: | 120 °C, 0 min |
| Detector: | FID |
| Sensitivity: | 128 x 10 ⁻¹² AFS |
| Injection Mode: | Split |

Components


1. Acetaldehyde
2. Ethyl Acetate
3. Methanol
4. Ethanol
5. Propan-1-ol
6. 2-Methylpropan-1-ol
7. 2-Methylbutan-1-ol + 3-Methylbutan-1-ol

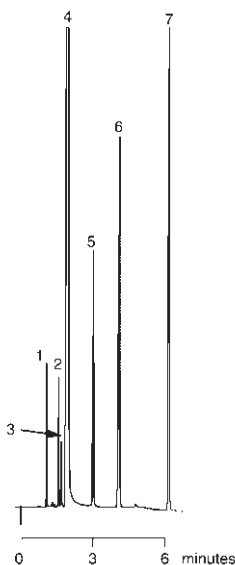

GC Columns and Applications

AN-0022-C | FAME Analysis with BPX90 – A Highly Polar Column

| | | | |
|-------------------------|---------------------------------------|-------------------|---------------------------|
| Column Part No.: | 054570 | Constant Flow: | ON |
| Phase: | 90% Cyanopropyl Polysilphenylsiloxane | Pressure: | 4.02 psi |
| Column Dimensions: | 15 m x 0.25 mm x 0.25 µm | Column Flow Rate: | 1.3 ml/min |
| Injector Temperature: | 250 °C | Linear Velocity: | 59 cm/sec |
| Injection Volume: | 1.0 µL | Initial Temp.: | 70 °C hold for 1 minute |
| Injector Type: | Split | Rate: | 20 °C/min to 150 °C |
| Split Ratio: | 100:1 | Rate: | 10 °C/min |
| Liner Type: | FocusLiner™ | Final Temp.: | 250 °C hold for 5 minutes |
| Carrier Gas: | Helium | Detector Type: | MSD |

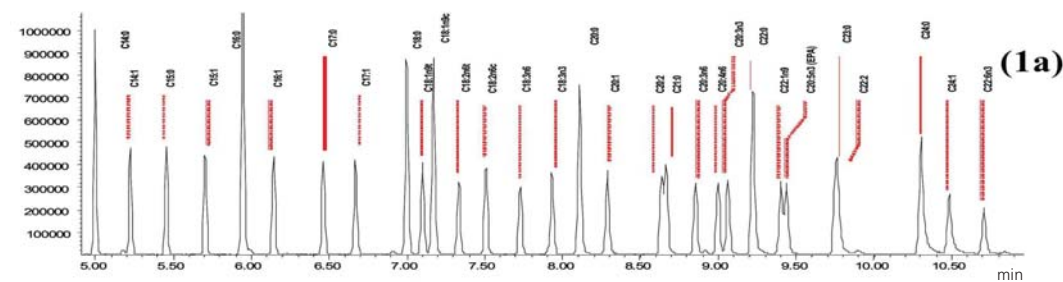




GC Columns and Applications

AN-0011-C | Analysis of Omega-3 Fatty Acids using a Highly Selective GC Capillary Column

| | |
|-------------------------|-----------------------------|
| Column Part No.: | 054606 |
| Phase: | BPX70, 0.25 µm film |
| Sample: | 10 ppm in methanol |
| Column: | 25 m x 0.32 mm ID |
| Initial Temp: | 80 °C, 2 min |
| Rate 1: | 50 °C/min to 130 °C, 10 min |
| Rate 2: | 2 °C/min to 172 °C |
| Final Temp: | 172 °C, 6 min |
| Detector Type: | FID |
| Detector Temp: | 300 °C |
| Carrier Gas: | He, 10 psi |

| | |
|--------------------------|---------------------|
| Carrier Gas Flow: | 2.2 mL/min |
| Constant Flow: | On |
| Average Linear Velocity: | 39 cm/sec at 80 °C |
| Injection Mode: | Split |
| Split Ratio: | 58:1 |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Autosampler: | No |
| Liner Type: | 4 mm ID FocusLiner™ |
| Liner Part No.: | 092002 |

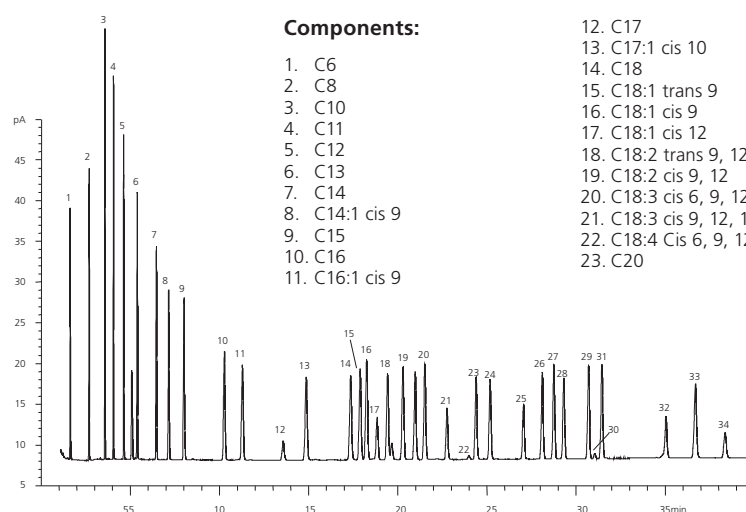

Components:

1. C6
2. C8
3. C10
4. C11
5. C12
6. C13
7. C14
8. C14:1 cis 9
9. C15
10. C16
11. C16:1 cis 9

12. C17
13. C17:1 cis 10
14. C18
15. C18:1 trans 9
16. C18:1 cis 9
17. C18:1 cis 12
18. C18:2 trans 9, 12
19. C18:2 cis 9, 12
20. C18:3 cis 6, 9, 12
21. C18:3 cis 9, 12, 15
22. C18:4 Cis 6, 9, 12, 15
23. C20


24. C21:1 cis 11
25. C20:2 cis 11,14
26. C20:3 cis 8, 11,14
27. C20:4 cis 5, 8, 11, 14
28. C20:3 cis 11, 14, 17
29. C22
30. C20:5 cis 5, 8, 11, 14, 17
31. C22:1 cis 13
32. C22:4 cis 7, 10, 13, 16
33. C24
34. C22:6 cis 4,7,10,13,16,19

Notes: The chromatogram shows the excellent separation of a complex mixture of FAME compounds. Note the excellent peak shape and separation of the Omega-1,2 and 3 fatty acid isomers both structural and cis and trans.


SGE would like to thank Masterfoods UK for supplying the sample and chromatographic conditions for this chromatogram.

FOO 16 | Analysis of Triglyceride Standards on HT5

| | |
|-------------------------|------------------------------------|
| Column Part No.: | 054661 |
| Phase: | HT5, 0.1 µm |
| Column: | 6 m x 0.53 mm I.D. (Aluminum Clad) |
| Initial Temp.: | 60 °C, 0 min |
| Program Rate: | 10 °C/min |
| Final Temp.: | 370 °C, 5 min |
| Carrier Gas: | H ₂ , 2 psi |
| Detector: | F.I.D. |
| Sensitivity: | 32 x 10 ⁻¹² AFS |
| Injection Mode: | On-column |

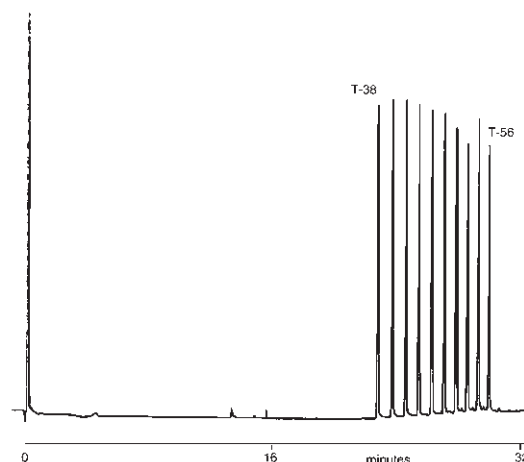

Notes: For the analysis of triglycerides, on-column injection is recommended. Temperatures above 380 °C are not recommended as triglycerides can degrade.

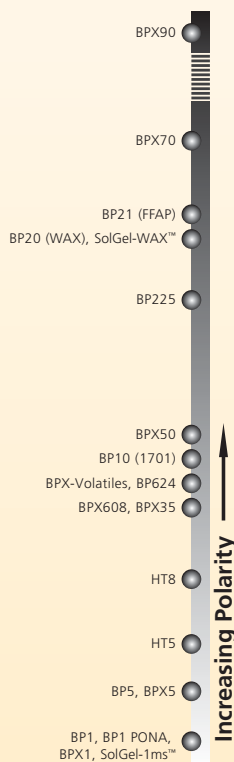


FLA 05 | Analysis of Menthol Oil on CYDEX-B

| | | | |
|-------------------------|-----------------------|-----------------|----------------|
| Column Part No.: | 054901 | Final Temp.: | 130 °C |
| Phase: | Cydex-B, 0.25 µm film | Carrier Gas: | H ₂ |
| Column: | 50 m x 0.22 mm I.D. | Detector: | F.I.D. |
| Initial Temp.: | 100 °C, 5 min | Sensitivity: | 32 x 10-12 AFS |
| Rate: | 2 °C/min | Injection Mode: | Split |



GC Columns and Applications

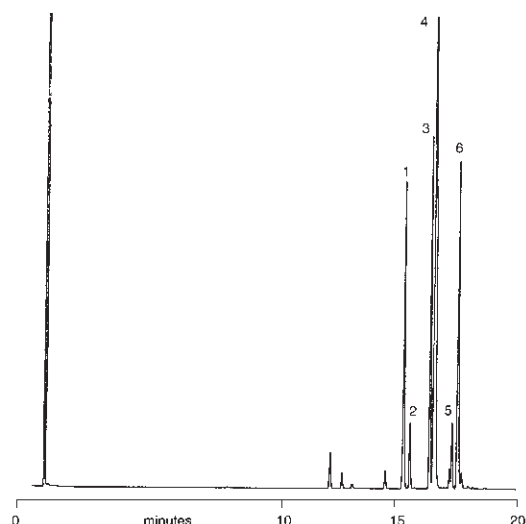


Components

1. (+) Neomenthol
2. (-) Neomenthol
3. (+) Menthol
4. (-) Menthol
5. (+) a-Terpineol
6. (-) a-Terpineol

Notes: Cydex - B column enables the separation of three different enantiomer pairs in Menthol Oil.

FLA 19 | Analysis of Eucalyptus Oil on SolGel-WAX™

| | | | |
|-------------------------|---------------------------|--------------------------|----------------------------|
| Column Part No.: | 054796 | Constant Flow: | On |
| Phase: | SolGel-WAX™, 0.25 µm film | Average Linear Velocity: | 35 cm/sec at 40 °C |
| Sample: | Neat | Injection Mode: | Split |
| Column: | 30 m x 0.25 mm ID | Split Ratio: | 100:1 |
| Initial Temp.: | 40 °C, 1 min. | Injection Volume: | 0.2 µL |
| Rate 1: | 8 °C/min to 220 °C, | Injection Temp.: | 250 °C |
| Final Temp: | 220 °C, 5 min. | Liner Type: | 4 mm ID Single Taper Liner |
| Detector Type: | Mass Spectrometer | Liner Part Number: | 092017 |
| Carrier Gas: | He, 25.7 psi | Full Scan / SIM: | Full scan 45-450 |
| Carrier Gas Flow: | 1.8 mL/min. | | |

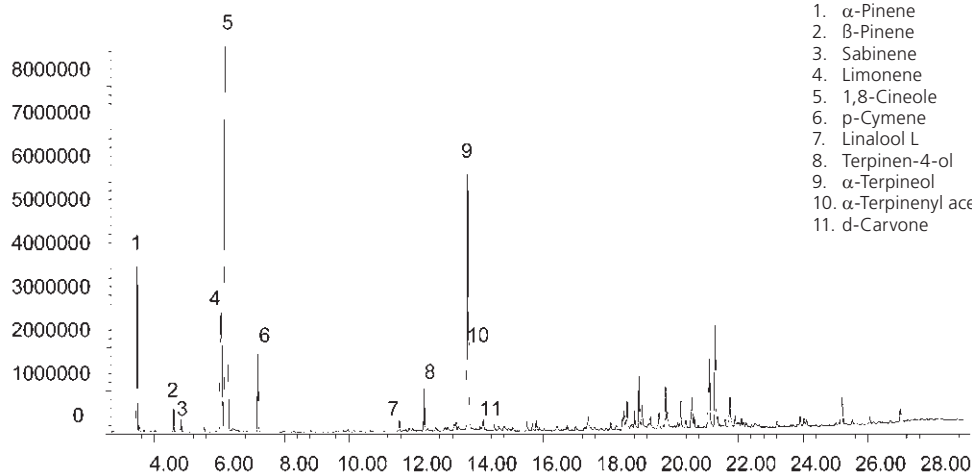

Components


1. α-Pinene
2. β-Pinene
3. Sabinene
4. Limonene
5. 1,8-Cineole
6. p-Cymene
7. Linalool L
8. Terpinen-4-ol
9. α-Terpineol
10. α-Terpinenyl acetate
11. d-Carvone





GC Columns and Applications

FOO 02 | Analysis of Food Additives Antimicrobials on BP5

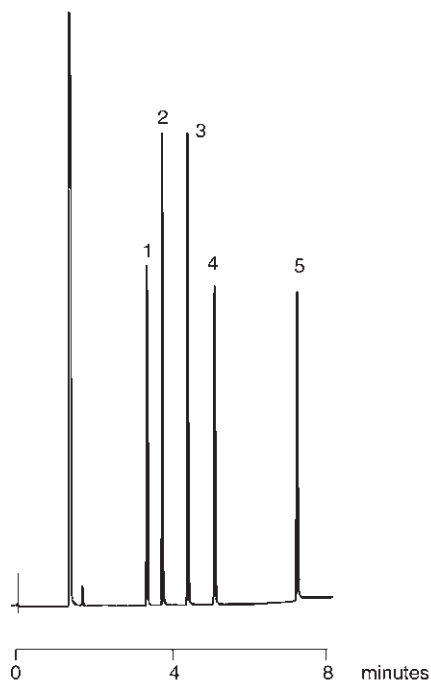

| | |
|-------------------------|-------------------|
| Column Part No.: | 054186 |
| Phase: | BP5, 0.5 µm film |
| Column: | 25 m x 0.32 mm ID |
| Initial Temp: | 160 °C, 0 min |
| Rate: | 15 °C/min |
| Final Temp: | 280 °C, 0 min |
| Detector: | FID |
| Sensitivity: | 256 x 10-12 AFS |
| Injection Mode: | Split |

Components



1. Methyl Paraben
2. Ethyl Paraben
3. Propyl Paraben
4. Butyl Paraben
5. Heptyl Paraben

FOO 04 | Analysis Of 13 Sugar Component Alditol Acetate Mixture on BPX70

| | |
|-------------------------|--|
| Column Part No.: | 054622 |
| Phase: | BPX70, 0.25 µm film |
| Column: | 30 m x 0.25 mm I.D. |
| Initial Temp.: | 190 °C, 1 min. |
| Program Rate: | 3 °C/min. |
| Final Temp: | 260 °C, 10min. |
| Carrier Gas: | He, 50 kPa |
| Detector: | MS (Electron Impact Ionisation, Ionisation Potential 70 eV) Scan 100 m/z to 350 m/z in 0.3 s. |
| Injection Mode: | Split 50:1 |

Components

1. Erythritol
2. 2-Deoxy-ribitol
3. Rhamnitol
4. Fucitol
5. Ribitol
6. Arabinitol
7. Xylitol
8. 2-Deoxy-glucitol
9. Allitol
10. Mannitol
11. Galacitol
12. Glucitol
13. Myo-inositol

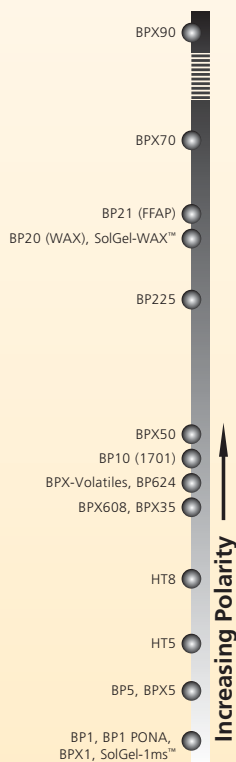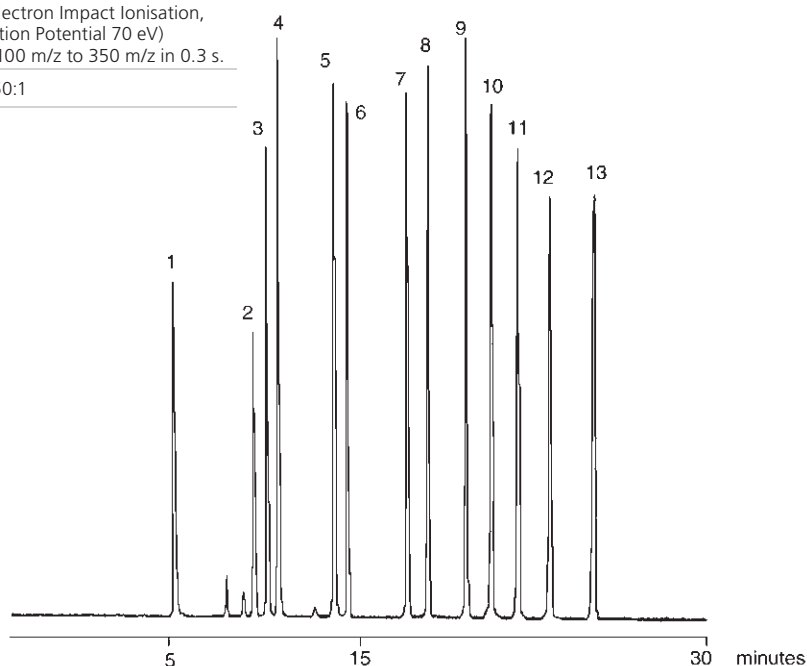


FOO 21 | Plant Sterols

| | |
|-------------------------|-------------------|
| Column Part No.: | 054148 |
| Phase: | BPX5, 1.0 µm |
| Column: | 30 m x 0.53 mm ID |
| Initial Temp.: | 320 °C |
| Detector: | FID, 360 °C |
| Injector Mode: | split 100:1 |
| Carrier Gas: | He, 3 psi |
| Injection Volume: | 1 µL |

Components

- | | |
|-------------------|---------------------|
| 1. Coprosterol | 7. Campesterol |
| 2. Cholesterol | 8. Stigmasterol |
| 3. Cholestanol | 9. Unknown |
| 4. Desmosterol | 10. beta-Sitosterol |
| 5. Brassicasterol | 11. Lanosterol |
| 6. Ergosterol | |

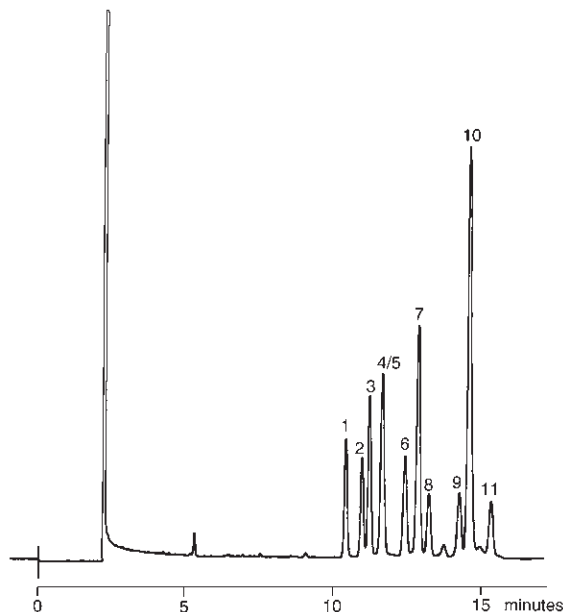


GC Columns and Applications

FOO 24 | Analysis of Wine on BP20

| | |
|-------------------------|------------------------|
| Column Part No.: | 054442 |
| Phase: | BP20, 1.0 µm |
| Column: | 25 m x 0.32 mm ID |
| Initial Temp.: | 40 °C, 2 min |
| Rate 1: | 5 °C/min |
| Temp 2: | 50 °C |
| Rate 2: | 15 °C/min |
| Final Temp.: | 190 °C |
| Carrier Gas: | H ₂ , 6 psi |
| Injection Mode: | 2 µL |

Components

- | | |
|------------------|--------------------|
| 1. Acetaldehyde | 6. Propanol |
| 2. Ethyl Acetate | 7. Isobutanol |
| 3. Methanol | 8. Isoamyl Alcohol |
| 4. Isopropanol | 9. Acetic Acid |
| 5. Ethanol | 10. Unknown |

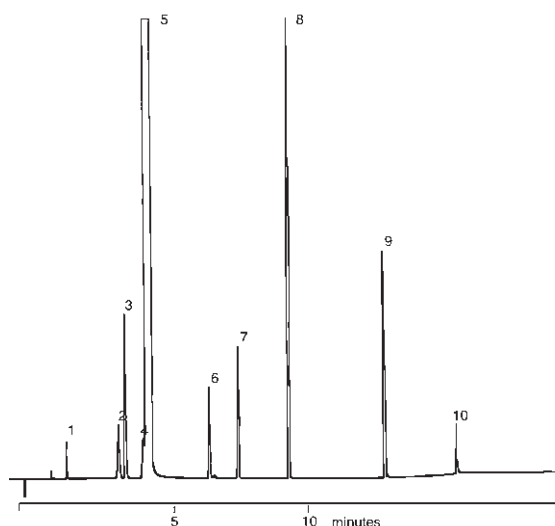




GC Columns and Applications

FLA 14 | Analysis of Lavender Oil on BPX5



| | |
|-------------------------|---------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.2 5 µm film |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp.: | 40 °C, 1 min |
| Rate 1: | 5 °C/min to 260 °C |
| Final Temp.: | 260 °C |
| Detector Type: | Mass Spectrometer |
| Carrier Gas: | He, 7.0 psi |
| Carrier Gas Flow: | 1.0 mL/min |
| Constant Flow: | On |

| | |
|--------------------------|----------------------------|
| Average Linear Velocity: | 36 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 200:1 |
| Purge on (Split) | |
| Vent Flow: | 200 mL/min |
| Injection Volume: | 0.2 µL |
| Injection Temp.: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

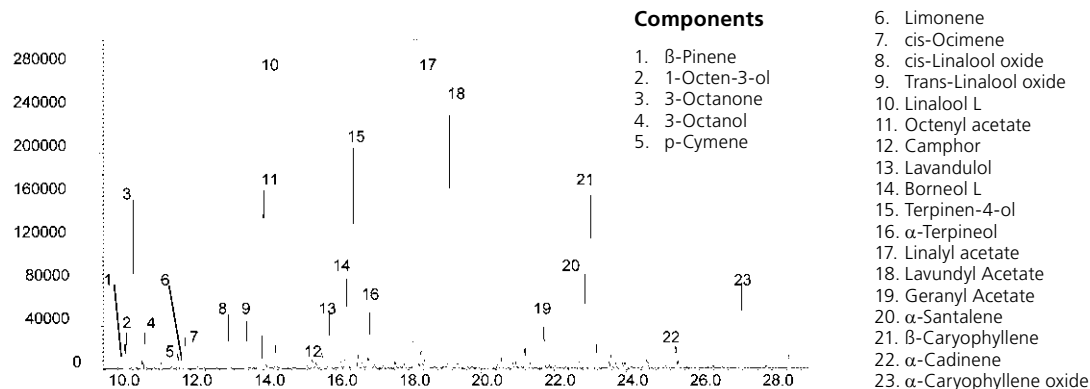

FLA 03 | Analysis of Orris Concentrate on BP20

| | |
|-------------------------|---------------------|
| Column Part No.: | 054436 |
| Column: | BP20, 0.5 µm |
| Phase: | 25 m x 0.32 mm I.D. |
| Initial Temp.: | 70 °C, 1 min |
| Rate: | 10 °C/min |
| Final Temp.: | 250 °C, 10 min |
| Carrier Gas: | Helium |
| Carrier Pressure: | 10 psi |
| Injection Mode: | Split 50:1 |

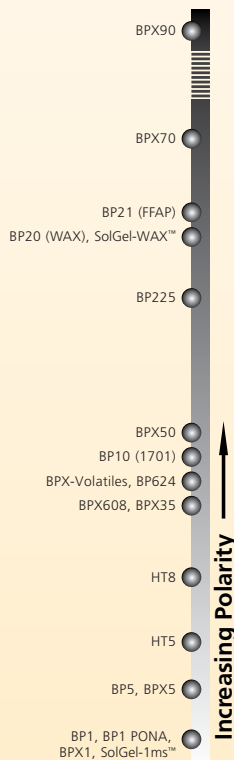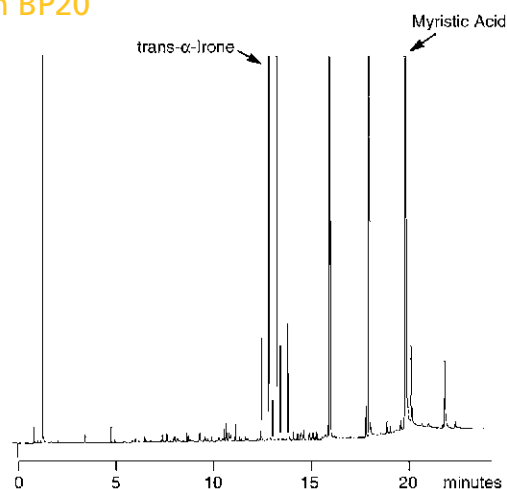


FLA 21 | Analysis of Spearmint Oil on SolGel-WAX™



GC Columns and Applications

| | | | |
|-------------------------|---------------------------|--------------------------|----------------------------|
| Column Part No.: | 054796 | Constant Flow: | On |
| Phase: | SolGel-WAX™, 0.25 µm film | Average Linear Velocity: | 35 cm/sec at 40 °C |
| Sample: | Neat | Injection Mode: | Split |
| Column: | 30 m x 0.25 mm ID | Split Ratio: | 100:1 |
| Initial Temp.: | 40 °C, 1 min. | Injection Volume: | 0.2 µL |
| Rate 1: | 8 °C/min to 220 °C | Injection Temp.: | 250 °C |
| Final Temp.: | 220 °C, 5 min. | Liner Type: | 4 mm ID Single Taper Liner |
| Detector Type: | Mass Spectrometer | Liner Part Number: | 092017 |
| Carrier Gas: | He, 25.7 psi | Full Scan / SIM: | Full scan 45-450 |
| Carrier Gas Flow: | 1.8 mL/min. | | |

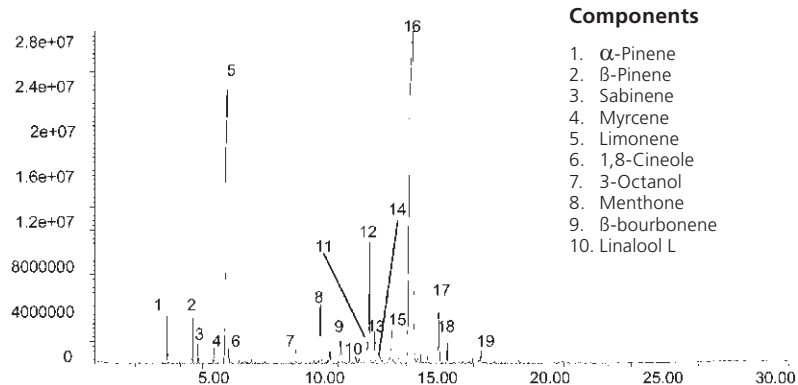


Components

- | | |
|------------------------|---------------------------------|
| 1. α -Pinene | 11. <i>trans</i> Caryophyllene |
| 2. β -Pinene | 12. <i>cis</i> dihydrocarvone |
| 3. Sabinene | 13. <i>trans</i> dihydrocarvone |
| 4. Myrcene | 14. Menthol |
| 5. Limonene | 15. Dihydrocarvyl acetate |
| 6. 1,8-Cineole | 16. L-Carvone |
| 7. 3-Octanol | 17. <i>trans</i> Carveol |
| 8. Menthone | 18. <i>cis</i> Carveol |
| 9. β -bourbonene | 19. Caryophyllene oxide |
| 10. Linalool L | |

FLA 18 | Analysis of Ylang Ylang Oil on SolGel-WAX™

| | | | |
|-------------------------|-----------------------|--------------------------|----------------------------|
| Column Part No.: | 054796 | Constant Flow: | On |
| Phase: | SolGel-WAX™, 0.25 µm | Average Linear Velocity: | 35 cm/sec at 40 °C |
| Sample: | Ylang Ylang oil neat. | Injection Mode: | Split |
| Column: | 30 m x 0.25 mm ID | Split Ratio: | 120:1 |
| Initial Temp.: | 40 °C, 2 min. | Injection Volume: | 0.1 µL |
| Rate 1: | 3 °C/min to 250 °C | Injection Temp.: | 250 °C |
| Final Temp.: | 250 °C, 10 min. | Autosampler: | No |
| Detector Type: | Mass Spectrometer | Liner Type: | 4 mm ID Double Taper Liner |
| Carrier Gas: | He, 25.7 psi | Liner Part Number: | 092018 |
| Carrier Gas Flow: | 1.8 mL/min. | Full Scan / SIM: | Full scan 45-450 |

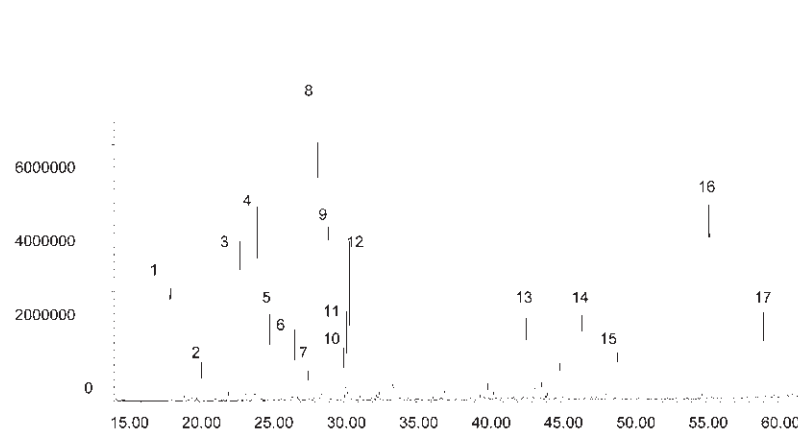

Components

1. p-Methyl anisole
2. α -Copaene
3. Linalool L
4. β -Caryophyllene
5. Methyl benzoate
6. α -Humulene
7. α -Amorphene
8. Germacrene
9. Benzyl acetate
10. δ -Cadinene
11. α -Farnesene
12. Geranyl acetate
13. *trans*-Cinamyl acetate
14. Farnesyl acetate
15. Farnesol
16. Benzyl benzoate
17. Benzyl salicylate






GC Columns and Applications

FLA 16 | Analysis of Pine Oil on BPX5

| | |
|-------------------------|--------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp.: | 40 °C, 1 min. |
| Rate 1: | 5 °C/min to 260 °C |
| Final Temp: | 260 °C |
| Detector Type: | Mass Spectrometer |
| Carrier Gas: | He, 7.0 psi |
| Carrier Gas Flow: | 1.0 mL/min. |
| Constant Flow: | On |

| | |
|--------------------------|----------------------------|
| Average Linear Velocity: | 36 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 200:1 |
| Purge on (Split) | |
| Vent Flow: | 200 mL/min. |
| Injection Volume: | 0.2 µL |
| Injection Temp.: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

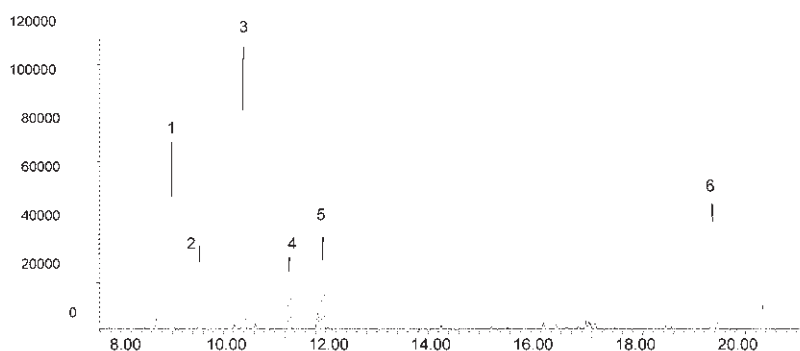


Components

1. α-Pinene
2. Camphene
3. β-Pinene
4. δ-3-Carene
5. Limonene
6. Endobornyl acetate

FLA 15 | Analysis of Tea Tree Oil on BPX5


| | |
|-------------------------|--------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp.: | 40 °C, 1 min. |
| Rate 1: | 5 °C/min to 200 °C |
| Final Temp: | 200 °C |
| Detector Type: | Mass Spectrometer |
| Carrier Gas: | He, 7.0 psi |
| Carrier Gas Flow: | 1.0 mL/min. |
| Constant Flow: | On |

| | |
|--------------------------|----------------------------|
| Average Linear Velocity: | 36 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 200:1 |
| Purge on (Split) | |
| Vent Flow: | 200 mL/min. |
| Injection Volume: | 0.2 µL |
| Injection Temp.: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

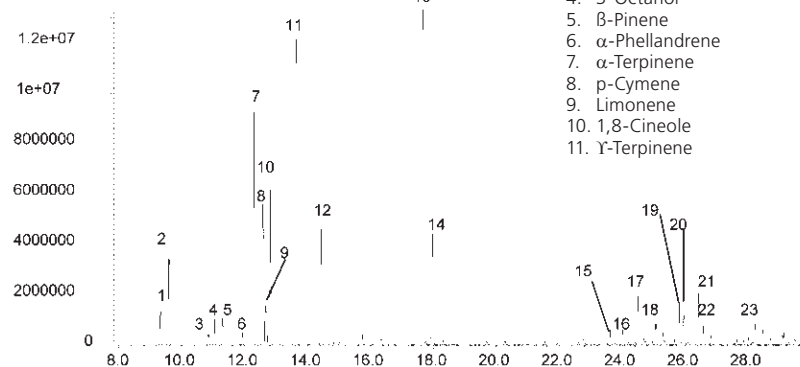

Components

- | | |
|-------------------|-----------------------------|
| 1. Thujene | 12. Terpinolene |
| 2. α-Pinene | 13. Terpinen-4-ol |
| 3. Sabinene | 14. α-Terpineol |
| 4. 3-Octanol | 15. α-Gurjunene |
| 5. β-Pinene | 16. (trans)-β-Caryophyllene |
| 6. α-Phellandrene | 17. Aromadendrene |
| 7. α-Terpinene | 18. Alloaromadendrene |
| 8. p-Cymene | 19. Ledene |
| 9. Limonene | 20. Germacrene B |
| 10. 1,8-Cineole | 21. δ-Cadinene |
| 11. γ-Terpinene | 22. 1s, cis-Calamenene |
| | 23. Globulol |

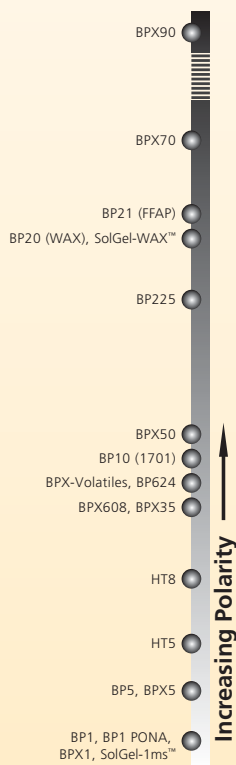

FLA 12 | Analysis of Nutmeg Oil on BPX5

| | |
|-------------------------|---------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp.: | 40 °C, 1 min. |
| Rate: | 5 °C/min to 260 °C, |
| Final Temp: | 260 °C |
| Detector Type: | Mass Spectrometer |
| Carrier Gas: | He, 7.0 psi |
| Carrier Gas Flow: | 1.0 mL/min. |


| | |
|-----------------------------|----------------------------|
| Constant Flow: | On |
| Average Linear Velocity: | 36 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 200:1 |
| Purge on (Split) Vent Flow: | 200 mL/min. |
| Injection Volume: | 0.2 µL |
| Injection Temp.: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |



GC Columns and Applications

Components

- | | |
|-------------------|----------------------------|
| 1. α-Thujene | 11. Limonene |
| 2. α-Pinene | 12. β-Phellandrene |
| 3. Camphene | 13. γ-Terpinene |
| 4. Sabinene | 14. trans-Sabinene hydrate |
| 5. β-Pinene | 15. α-Terpinolene |
| 6. Myrcene | 16. Terpinen-4-ol |
| 7. α-Phellandrene | 17. 1-α-Terpineol |
| 8. δ-3-Carene | 18. Safrole |
| 9. α-Terpinene | 19. α-Copaene |
| 10. p-Cymene | 20. Myristicin |
| | 21. Elemicin |

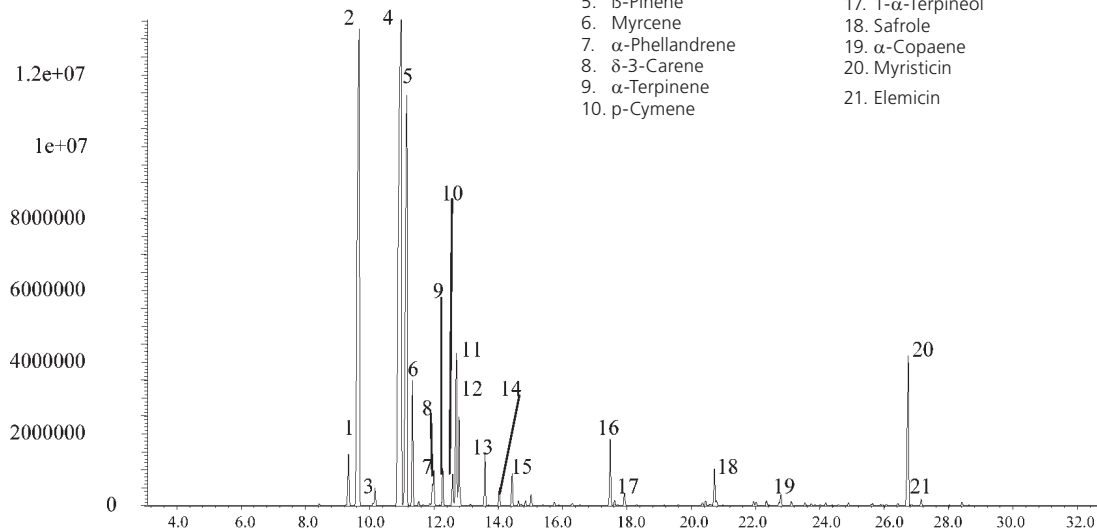




GC Columns and Applications

FLA 13 | Analysis of Rosemary Oil on BPX5


| | |
|-------------------------|---------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp.: | 40 °C, 1 min. |
| Rate 1: | 5 °C/min to 260 °C, |
| Final Temp: | 260 °C |
| Detector Type: | Mass Spectrometer |
| Carrier Gas: | He, 7.0 psi |
| Carrier Gas Flow: | 1.0 mL/min. |
| Constant Flow: | On |

| | |
|--------------------------|----------------------------|
| Average Linear Velocity: | 36 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 200:1 |
| Purge on (Split) | |
| Vent Flow: | 200 mL/min. |
| Injection Volume: | 0.2 µL |
| Injection Temp.: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

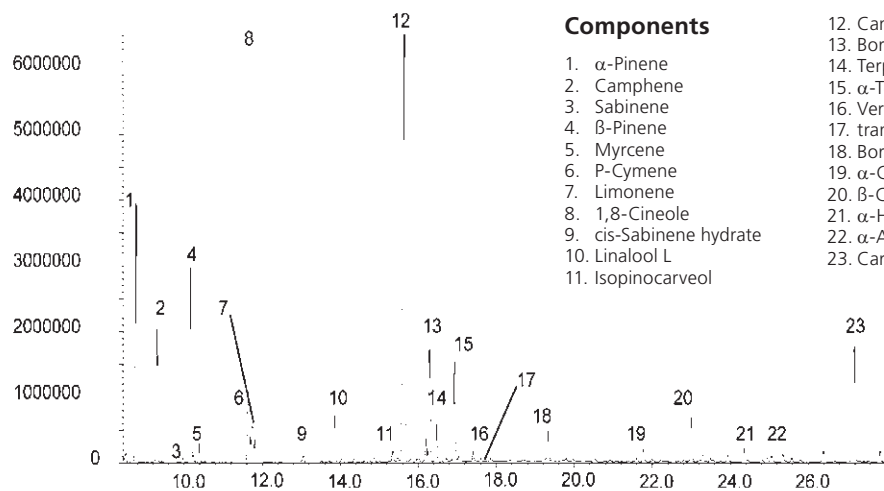

Components

- | | |
|-------------------------|-------------------------|
| 1. α-Pinene | 12. Camphor |
| 2. Camphene | 13. Borneol L |
| 3. Sabinene | 14. Terpinen-4-ol |
| 4. β-Pinene | 15. α-Terpineol |
| 5. Myrcene | 16. Verbenone |
| 6. p-Cymene | 17. trans-(+)-Carveol |
| 7. Limonene | 18. Bornyl acetate |
| 8. 1,8-Cineole | 19. α-Copaene |
| 9. cis-Sabinene hydrate | 20. β-Caryophyllene |
| 10. Linalool L | 21. α-Humulene |
| 11. Isopinocarveol | 22. α-Amorphene |
| | 23. Caryophyllene oxide |

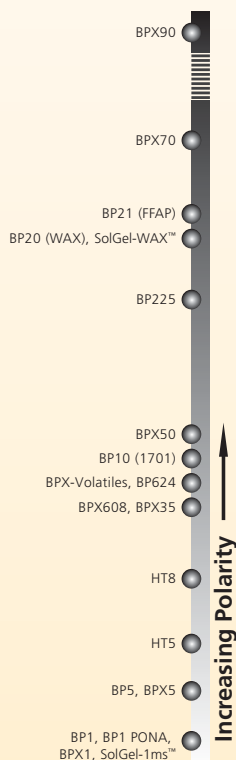


FLA 22 | Analysis of Tasmanian Lavender Oil on SolGel-WAX™



GC Columns and Applications

| | | | |
|-------------------------|---------------------------|--------------------------|----------------------------|
| Column Part No.: | 054796 | | |
| Phase: | SolGel-WAX™, 0.25 µm film | Constant Flow: | On |
| Sample: | Neat | Average Linear Velocity: | 35 cm/sec at 40 °C |
| Column: | 30 m x 0.25 mm ID | Injection Mode: | Split |
| Initial Temp.: | 40 °C, 1 min. | Split Ratio: | 100:1 |
| Rate 1: | 8 °C/min to 220 °C, | Injection Volume: | 0.2 µL |
| Final Temp: | 220 °C, 5 min. | Injection Temp.: | 250 °C |
| Detector Type: | Mass Spectrometer | Liner Type: | 4 mm ID Single Taper Liner |
| Carrier Gas: | He, 25.7 psi | Liner Part Number: | 092017 |
| Carrier Gas Flow: | 1.8 mL/min. | Full Scan / SIM: | Full scan 45-450 |

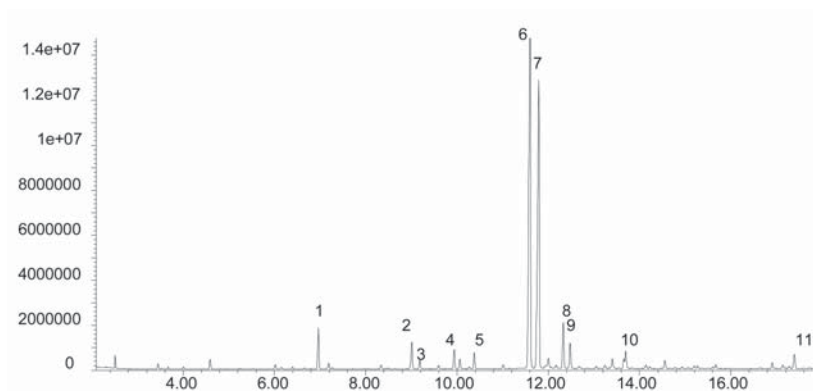

Components

1. 3-Octanone
2. Octenyl acetate
3. Octanol
4. Cis Linalool oxide
5. Trans Linalool Oxide
6. Linalool L
7. Linalyl acetate
8. Terpinen-4-ol
9. Lavandulyl acetate
10. Borneol L
11. Caryophyllene oxide





GC Columns and Applications


ENV 54 | Total Recoverable Petroleum Hydrocarbons (TRPH) Analysis on Standard and Fast BPX5

| | |
|-----------------------------|---------------------------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| TRPH (C8-C40): | 5 ng/ µL in dichloromethane |
| Initial Temp: | 40 °C , 2 min |
| Rate 1: | 30 °C/min to 330 °C |
| Rate 2: | N/A |
| Final Temp.: | 330 °C, 9 min |
| Detector Type: | FID, 350 °C |
| Carrier Gas: | He, 14.1 psi |
| Carrier Gas Flow : | 1.29 mL/min |
| Constant Flow: | On |
| Average Linear Velocity: | 40 cm/sec at 40 °C |
| Injection Mode: | Split, 120:1 |
| Purge On Time: | N/A |
| Purge On (Split) Vent Flow: | 160 mL/min |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Autosampler: | Yes |
| Liner Type : | 4 mm ID FocusLiner™ with single taper |
| Liner Part Number: | 092003 |

| | |
|-----------------------------|-----------------------------|
| Column Part Number: | 054099 |
| Phase: | BPX5, 0.10 µm film |
| Column: | 10 m x 0.10 mm ID |
| TRPH (C8-C40) Standard: | 5 ng/ µL in dichloromethane |
| Initial Temp.: | 40 °C , 1 min |
| Rate 1: | 30 °C/min to 330 °C |
| Rate 2: | N/A |
| Final Temp: | 330 °C, 0 min |
| Detector Type: | FID, 350 °C |
| Carrier Gas: | He, 28 psi |
| Carrier Gas Flow : | 0.52 mL/min |
| Constant Flow: | On |
| Average Linear Velocity: | 55 cm/sec at 40 °C |
| Injection Mode: | Split, 120:1 |
| Purge On Time: | N/A |
| Purge On (Split) Vent Flow: | 62 mL/min |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Autosampler: | Yes |
| Liner Type : | 2.3 mm ID FocusLiner™ |
| Liner Part Number: | 092005 |



NORMAL

Chromatogram showing separation of Total Recoverable Petroleum Hydrocarbons using a conventional 30 meter x 0.25 mm ID BPX5 column with a 0.25 micron film.

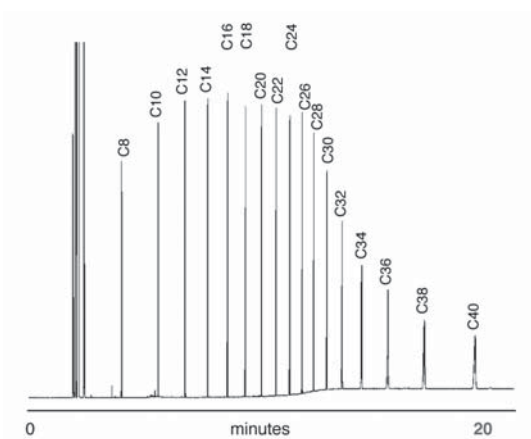

FAST

Chromatogram showing separation of Total Recoverable Petroleum Hydrocarbon using a FAST BPX5 column.

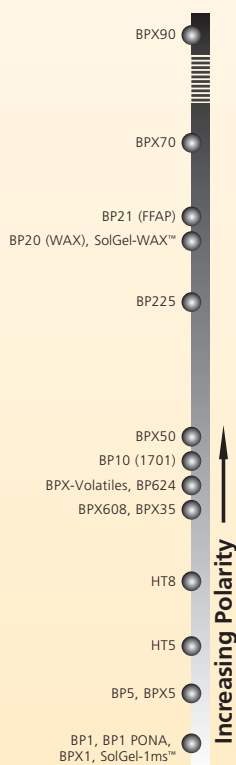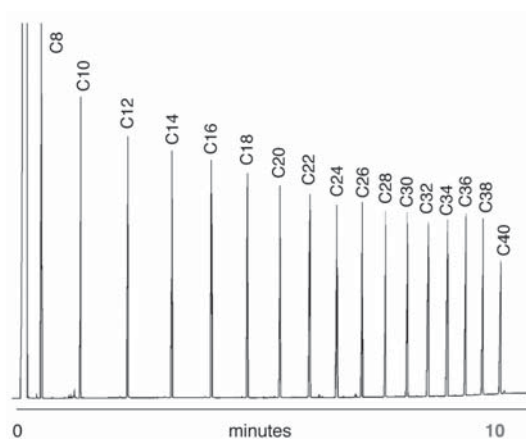


PET 01 | Analysis of Gasoline Range Hydrocarbons on BP1-PONA



GC Columns and Applications

| | | | |
|-------------------------|-------------------|-----------------|-------------------------|
| Column Part No.: | 054950 | Temp. 3: | 120 °C |
| Phase: | BP1 PONA | Rate 3: | 10 °C/min |
| Column: | 50 m x 0.15 mm ID | Final Temp.: | 190 °C |
| Initial Temp.: | 30 °C, 5 min hold | Detector: | FID |
| Rate 1: | 2 °C/min | Sensitivity: | 32 x 10-12 AFS |
| Temp. 2: | 80 °C | Injection Mode: | Split |
| Rate 2: | 50 °C/min | Carrier Gas: | H ₂ , 40 psi |

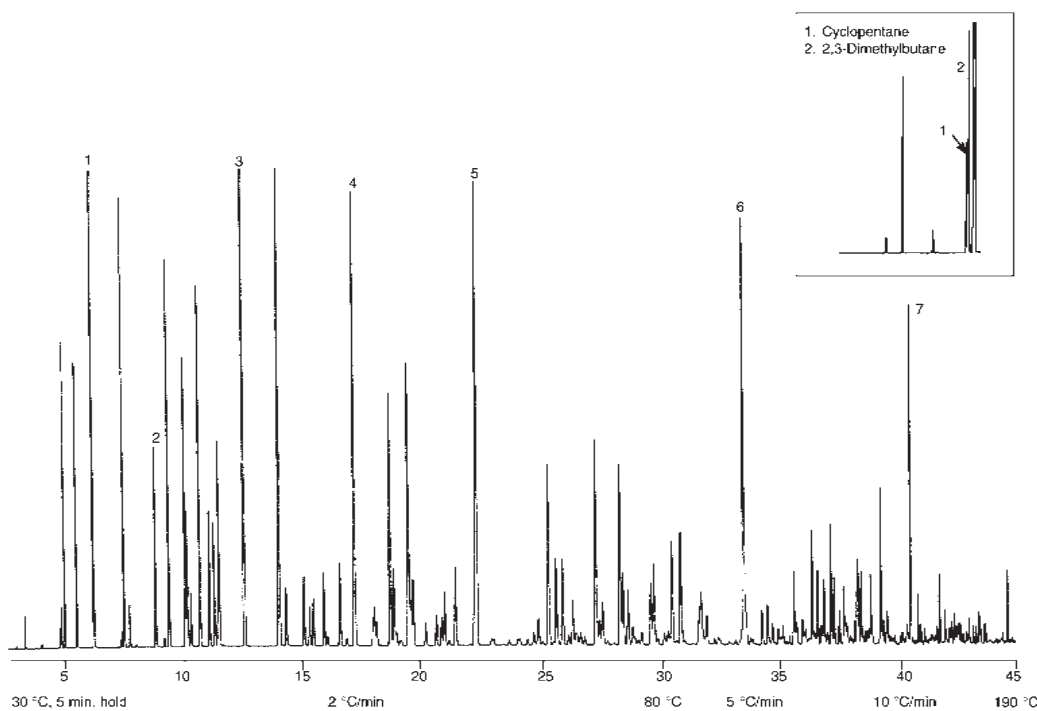

Components

| TIME | COMPOUND |
|-------|---|
| 4.85 | Cyclopentane |
| 5.00 | 2,3-Dimethylbutane |
| 5.25 | 2-Methylpentane |
| 5.74 | 3-Methylpentane |
| 6.45 | n-Hexane |
| 7.46 | 2,2-Dimethylpentane |
| 7.60 | Methylcyclopentane |
| 7.91 | 2,4-Dimethylpentane |
| 8.18 | 2,2,3-Trimethylbutane |
| 8.99 | Benzene |
| 9.35 | 3,3-Dimethylpentane |
| 9.55 | Cyclohexane |
| 10.23 | 2-Methylhexane |
| 10.32 | 2,3-Dimethylpentane |
| 10.47 | 1,1-Dimethylcyclohexane |
| 10.83 | 3-Methylhexane |
| 11.23 | 1-trans-3-Dimethylcyclopentane |
| 11.43 | 1-cis-3-Dimethylcyclopentane |
| 11.55 | 3-Ethylpentane |
| 11.63 | 1-trans-2-Dimethylcyclopentane |
| 11.78 | 2,2,4-Trimethylpentane |
| 12.73 | n-Heptane |
| 14.23 | Methylcyclohexane |
| 14.53 | 2,2-Dimethylhexane |
| 15.27 | Ethylcyclopentane |
| 15.49 | 2,5-Dimethylhexane |
| 15.65 | 2,4-Dimethylhexane |
| 16.09 | 1-trans-2-cis-4-Trimethylcyclopentane |
| 16.24 | 2,3,4-Trimethylpentane |
| 16.78 | 1-trans-2-cis-3-Trimethylcyclopentane |
| 17.05 | 2,3,3-Trimethylpentane |
| 17.39 | Toluene |
| 18.27 | 2,3-Dimethylhexane |
| 18.43 | 2-Methyl-3-ethylpentane |
| 18.84 | 2-Methylheptane |
| 19.69 | 1-Methyl-2-ethylcyclopentane |
| 18.98 | 4-Methylheptane |
| 19.23 | 1-cis-2-cis-4-trans-Trimethylcyclopentane |
| 19.50 | 3-Methylheptane |
| 19.77 | 1-trans-4-Dimethylcyclohexane |
| 20.73 | 1-Methyl-cis-2-ethylcyclopentane |
| 20.86 | 1-Methyl-trans-3-ethylcyclopentane |
| 21.08 | 1-Methyl-cis-3-ethylcyclohexane |
| 21.27 | 1-Ethyl-1-methylcyclopentane |
| 21.53 | 1-trans-2-Dimethylcyclohexane |
| 22.43 | n-Octane |
| 23.05 | iso-Propylcyclopentane |
| 24.14 | 2.2.5-Trimethylhexane |
| 24.19 | 2,2,4-Trimethylhexane |
| 24.53 | 2,4,4-Trimethylhexane |
| 24.79 | 2,3,5-Trimethylhexane |
| 25.16 | 2,4-Dimethylheptane |
| 25.41 | n-Propylcyclopentane |
| 25.73 | 1-cis-2-Dimethylcyclohexane |
| 26.00 | 1,1,3-Trimethylcyclohexane |
| 26.25 | 2,5-Dimethylheptane |
| 26.44 | 3,3-Dimethylheptane |
| 26.58 | 3,5-Dimethylheptane |
| 26.77 | 4,4-Dimethylheptane |
| 26.94 | 2,3,3-Trimethylhexane |
| 27.43 | Ethylbenzene |
| 27.57 | 1-cis-3-cis-5-Trimethylpentane |
| 27.69 | 1,1,4-Trimethylcyclohexane |
| 27.88 | 2,3,4-Trimethylhexane |
| 28.15 | 3,3,4-Trimethylhexane |
| 28.42 | m-Xylene |
| 28.54 | p-Xylene |
| 28.74 | 2,3-Dimethylheptane |
| 28.84 | 1-cis-2-trans-4-trans-Trimethylcyclohexane |
| 28.95 | 1-cis-2-trans-4-cis-Trimethylcyclohexane |
| 29.16 | 3,4-Dimethylheptane |
| 29.31 | 3-Methylethylhexane |
| 29.68 | 4-Methyloctane |
| 29.81 | 2-Methyloctane |
| 30.56 | 3-Methyloctane |
| 30.93 | o-Xylene |
| 31.75 | 1-Methyl-2-propylcyclopentane and 1-Methyl-trans-4-ethylcyclohexane |
| 31.98 | 1-Methyl-cis-4-ethylcyclohexane |
| 32.46 | 3,3-Diethylpentane |
| 32.89 | 2,2,6-Trimethylheptane |
| 33.17 | 1,1,2-Trimethylcyclohexane |
| 33.52 | n-Nonane |
| 34.26 | iso-Propylbenzene |
| 34.48 | tert-Butylcyclopentane |
| 34.68 | tert-Butylbenzene |
| 35.57 | sec-Butylcyclopentane |
| 36.33 | 3-Methylnonane |
| 36.56 | n-Propylbenzene |
| 36.83 | n-Propylcyclohexane |
| 37.12 | m-Ethyltoluene |
| 37.24 | p-Ethyltoluene |
| 37.64 | 1,3,5-Trimethylbenzene |
| 38.20 | 2-Methylnonane |
| 38.36 | o-Ethyltoluene |
| 38.75 | 3,6-Dimethyloctane |
| 38.75 | 1,2,4-Trimethylbenzene |
| 40.32 | n-Decane |
| 40.63 | 1,2,3-Trimethylbenzene |
| 41.57 | 4-Methyldecane |
| 41.94 | sec-Butylbenzene |
| 42.45 | n-Butylbenzene |
| 44.54 | n-Undecane |






GC Columns and Applications

PET 11 | Analysis of Crude Oil and Wax Mixtures on HT5

| | | | |
|-------------------------|--|-----------------|----------------------------|
| Column Part No.: | 054635 | Final Temp.: | 480 °C |
| Phase: | HT5, 0.1 µm | Carrier Gas: | H ₂ , 15 psi |
| Column: | 12 m x 0.22 mm I.D. (Aluminum Clad) | Detector: | F.I.D. |
| Initial Temp.: | 35 °C | Sensitivity: | 32 x 10 ⁻¹² AFS |
| Program Rate: | 10 °C/min. | Injection Mode: | Split |

Notes: HT5 is the best column for the analysis of hydrocarbons C₁₀ - C₇₀.


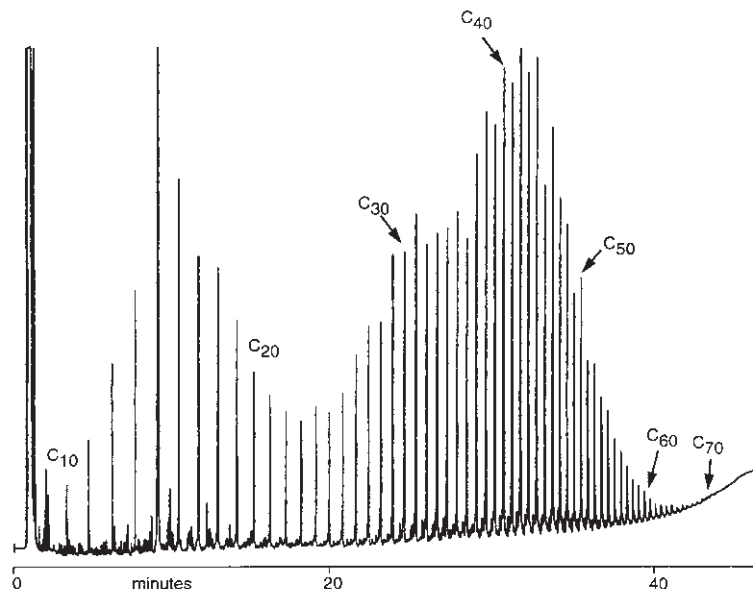


PET 26 | Standard for D2887 on BPX1

| | | | |
|-------------------------|--------------------|-----------------|---------------|
| Column Part No.: | 054802 | Final Temp.: | 350 °C, 10min |
| Phase: | BPX1, 2.65 µm film | Detector Temp.: | 400 °C |
| Column: | 10 m x 0.53 mm ID | Carrier Gas: | He, 20 mL/min |
| Initial Temp.: | 40 °C | Instrument: | HP 6890 |
| Rate: | 15 °C/min | | |

Separation Systems Injector

| | |
|----------------|----------------|
| Initial Temp.: | 80 °C |
| Rate: | 15 °C/min |
| Final Temp.: | 350 °C, 10 min |

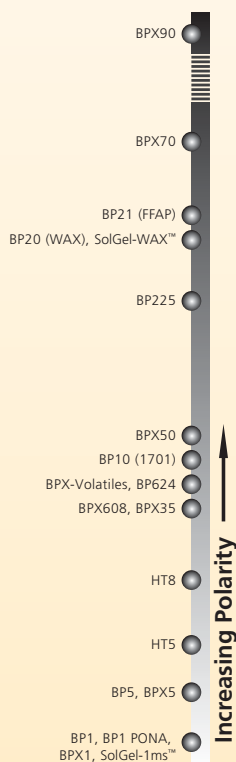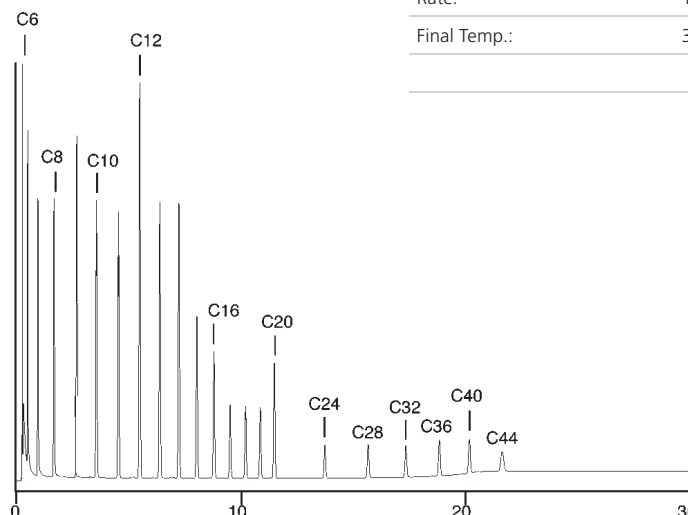

ENV 51 | Total Recoverable Petroleum Hydrocarbons (TRPH) C8-C40 on SolGel-1ms™

| | | | |
|-------------------------|---|------------------|--------------------|
| Column Part No.: | 054795 | | |
| Phase: | SolGel-1, 0.25 µm film 30 m x 0.25 mm ID | Pressure: | 16.6 psi |
| Sample Introduction: | Split / Splitless | Column Flow: | 1.6 mL/min |
| Injector Temp.: | 250 °C | Linear Velocity: | 35 cm/sec at 40 °C |
| Injection Volume: | 0.5 µL | Initial Temp: | 40 °C |
| Autosampler Syringe: | 5 µL Fixed Needle Part No. 001810 | Initial Time: | 2 min |
| Septa: | Auto-Sep T™ Part No. 041882 | Rate 1: | 30 °C/min |
| Injection Type: | Split | Final Temp.1: | 310 °C |
| Purge On Time: | NA | Hold Time: | 0 min |
| Purge On (Spilt) Vent: | 100 mL/min | Rate 2: | 10 °C/min |
| Split Ratio: | 62.5 to 1 | Final Temp. 2: | 340 °C |
| Liner Type: | Double taper Part No. 092018 | Hold Time: | 0 min |
| Carrier Gas: | He | Run Time: | 22.00 min |
| Constant Flow: | On | Detector Type: | FID at 340 °C |




GC Columns and Applications


Sample Description: TRPH mix 500 mg/L, 4 ng per component on column.

Components

1. C8
2. C10
3. C12
4. C14
5. C16
6. C18
7. C20
8. C22
9. C24
10. C26
11. C28
12. C30
13. C32
14. C34
15. C36
16. C38
17. C40

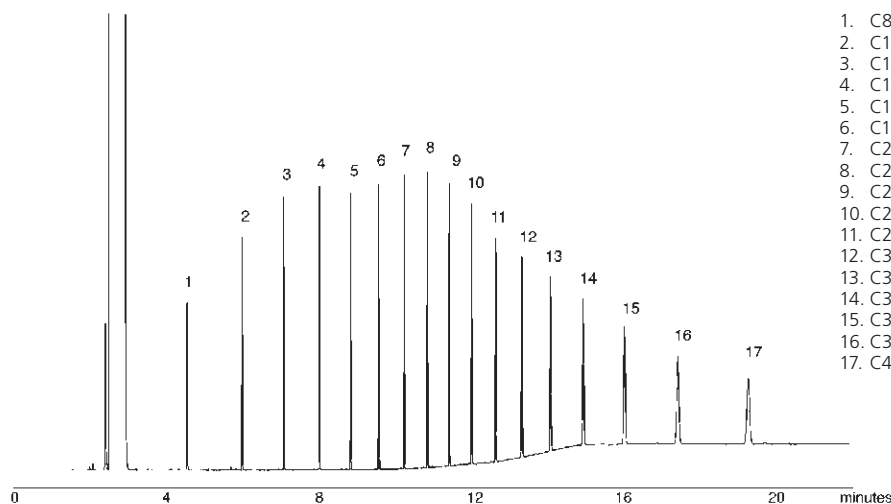

PET 27 | Analysis of Polywax 1000 on an Aluminum Clad HT5

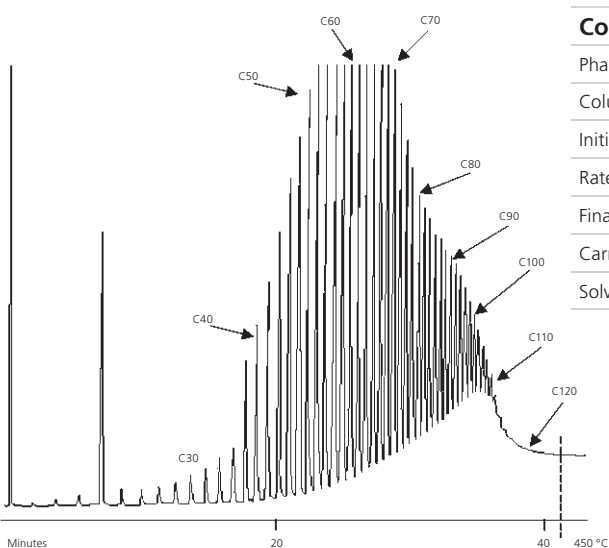


| | |
|-------------------------|--------------------|
| Column Part No.: | 054673 |
| Phase: | HT5, 0.075 µm film |
| Column: | 5 m x 0.53 mm ID |
| Initial Temp.: | 40 °C, 1 min |
| Rate: | 10 °C/min |
| Final Temp.: | 450 °C, 10 min |
| Carrier Gas: | He, 20 mL/min |
| Solvent: | CS ₂ |






GC Columns and Applications

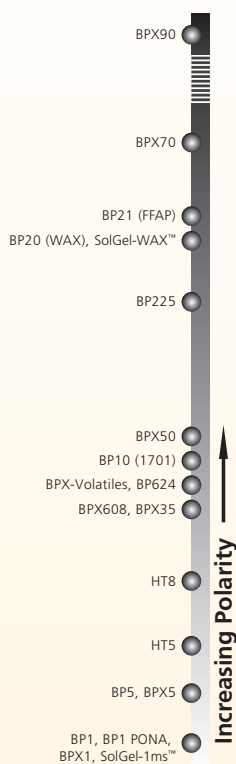

PET 22 | Unleaded Gasoline on BPX5

| | |
|-------------------------|--|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Sample Introduction: | Split / Splitless |
| Injector Temp.: | 240 °C |
| Injection Volume: | 0.1 µL |
| Autosampler Syringe: | 0.5 µL Removable Needle Part No. 000410 |
| Septa: | Auto-Sep T™ Part No. 041882 |
| Injection Type: | Split |
| Purge On Time: | NA |
| Purge On (Split) Vent: | 200 mL/min |
| Split Ratio: | 149 to 1 |
| Liner Type: | FocusLiner™ single taper Part No. 092003 |
| Carrier Gas: | He |

| | |
|------------------|--------------------|
| Constant Flow: | On |
| Pressure: | 13.6 psi |
| Column Flow: | 1.34 mL/min |
| Linear Velocity: | 30 cm/sec at 25 °C |
| Initial Temp.: | 25 °C |
| Initial Time: | 1 min |
| Rate 1: | 30 °C/min |
| Final Temp. 1: | 240 °C |
| Hold Time: | 1 min |
| Run Time: | 9.17 min |
| Final Temp. 2: | 340 °C |
| Hold Time: | 0 min |
| Run Time: | 22.00 min |
| Detector Type: | FID at 280 °C |

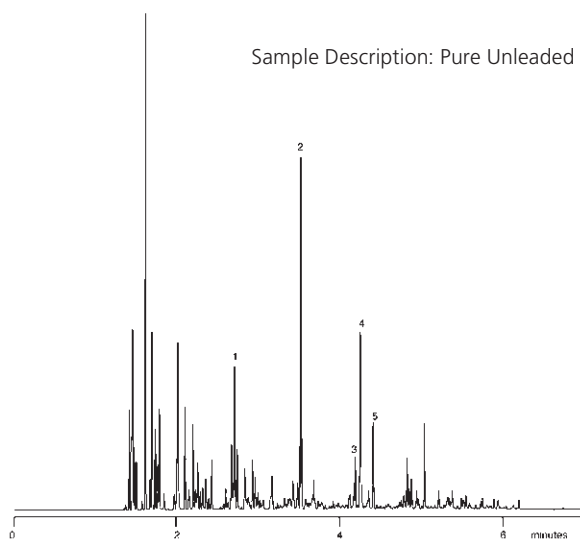

Sample Description: Pure Unleaded Gasoline


Components

1. Benzene
2. Toluene
3. Ethylbenzene
4. m, p - Xylene
5. o - Xylene

PET 18 | Analysis of Polywax 655 on Megabore BPX1

| | |
|-------------------------|------------------|
| Column Part No.: | 054800 |
| Phase: | BPX1, 0.1 µm |
| Column: | 5 m x 0.53 mm ID |
| Initial Temp: | 40 °C |
| Rate: | 15 °C |

| | |
|----------------|-----------------|
| Final Temp: | 420 °C, 5 min |
| Detector Temp: | 440 °C |
| Carrier: | He, 10 mL/min |
| Instrument: | HP 6890 |
| Solvent: | CS ₂ |

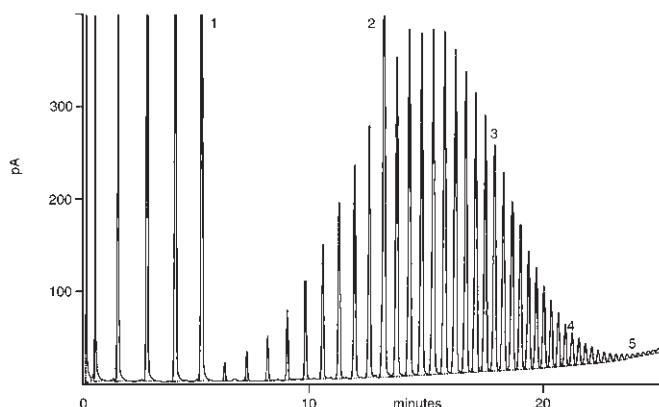



PET 06 | Analysis of Polywax 655 and Refinery Lubrication Oil on HT5



GC Columns and Applications

| | |
|-------------------------|------------------|
| Column Part No.: | 054661 |
| Phase: | HT5, 0.1 µm |
| Column: | 6 m x 0.53 mm ID |
| Initial Temp.: | 50 °C |
| Rate: | 10 °C/min |
| Final Temp.: | 480 °C, 15 min |

| | |
|-----------------|----------------------------|
| Detector: | FID |
| Sensitivity: | 40 x 10 ⁻¹² AFS |
| Injection Mode: | On-Column |
| Carrier Gas: | Hydrogen, 20 ml/min |
| Solvent: | CS ₂ |

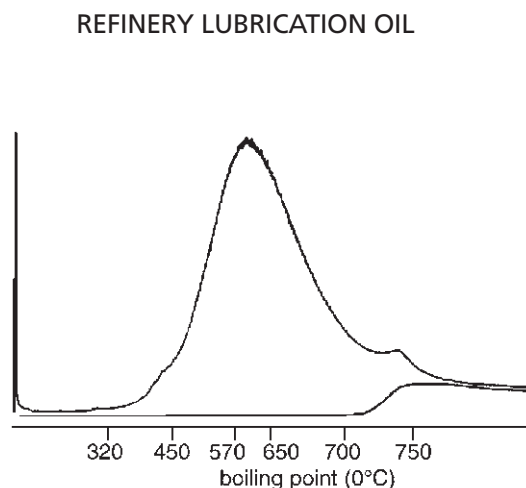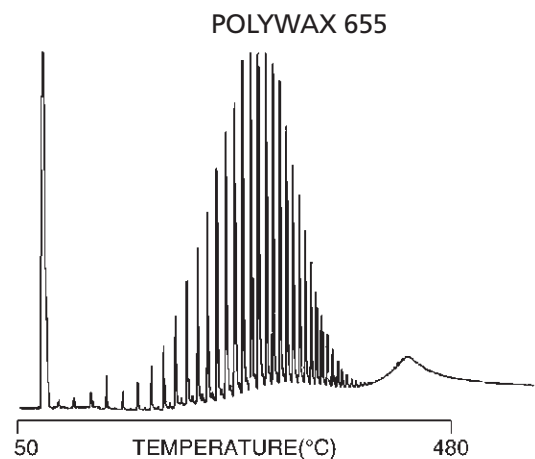

ENV 54 | BPX1 A New Era in Simulated Distillation Technology (SimD)

| | |
|------------------------|------------------|
| Column Part No: | 054800 |
| Phase: | BPX1, 0.1 µm |
| Column: | 5 m x 0.53 mm ID |
| Initial Temp.: | 40 °C |
| Rate: | 15 °C |
| Final Temp.: | 420 °C, 5 min. |

| | |
|----------------|-------------------|
| Detector Temp: | 440 °C |
| Carrier Gas: | Helium, 10 mL/min |
| Instrument: | HP6890 |
| Initial Temp.: | 40 °C |
| Rate: | 15 °C |
| Final Temp.: | 420 °C, 5 min. |

Data supplied by Dr. J. Lubkowitz and the staff at Separation Systems Inc.

Figure. 1. Standard mix for HTSD using BPX1-SimD


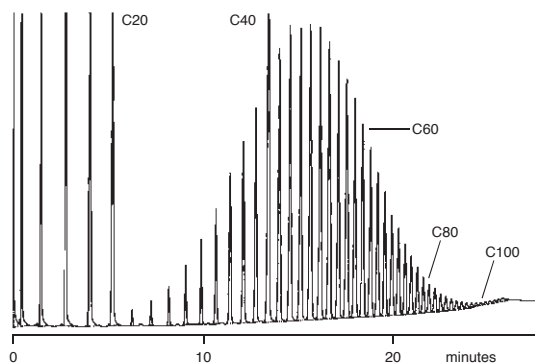


Figure. 2. Enlarged section of Figure 1.



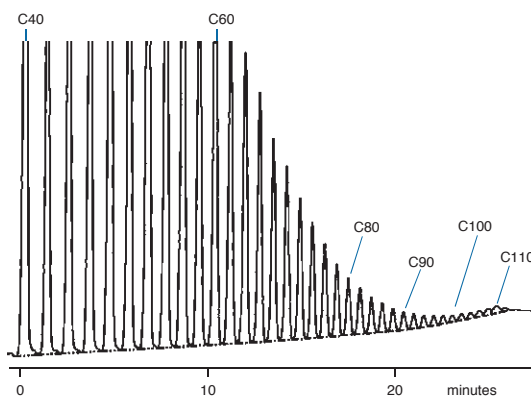

GC Columns and Applications

ALC 02 | Analysis of 18 Alcohols on BP20

Column Part No.: 054427

Phase: BP20, 0.25 µm film

Column: 30 m x 0.25 mm ID

Initial Temp: 45 °C, 2 min



Rate: 3 °C/min

Final Temp: 80 °C, 0 min

Detector: FID

Sensitivity: 128 x 10⁻¹² AFS

Injection Mode: Split

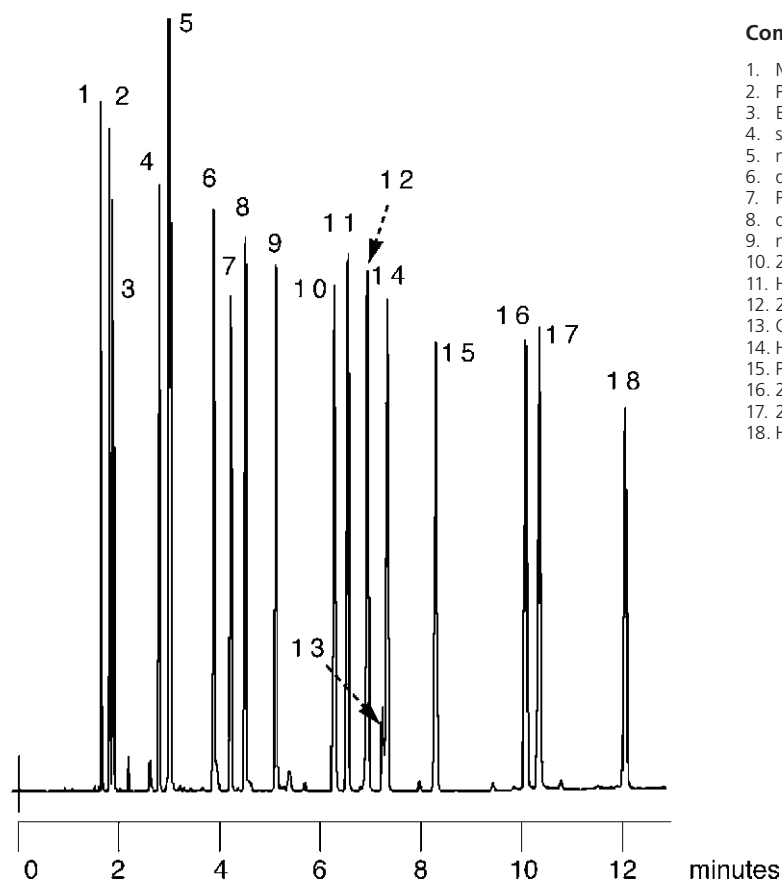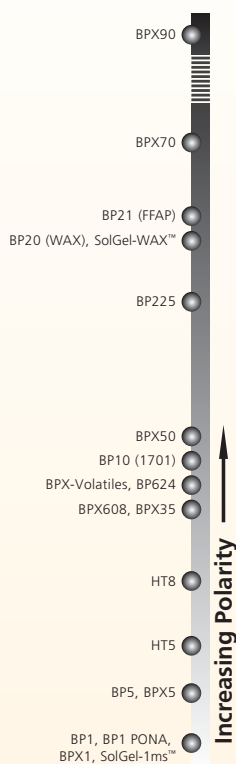

Components


1. Methanol
2. Propan-2-ol
3. Ethanol
4. sec-Butan-1-ol
5. n-Propanol + 2-Methyl-3-Buten-2-ol
6. d,l-3-Methyl-2-Butan-1-ol
7. Pentan-3-ol
8. d,l-2-Pentan-1-ol
9. n-Butanol
10. 2,4-Dimethyl, Pentan-3-ol
11. Hexan-3-ol
12. 2-Methyl Prop-2-en-1-ol
13. Crotyl Alcohol (2-Buten-1-ol)
14. Hexan-2-ol
15. Pentan-1-ol
16. 2-Methyl Pentan-1-ol
17. 2-Ethyl Butan-1-ol
18. Hexan-1-ol

ACI 03 | Analysis of 11 Organic Acids on BP20

| | | | |
|-------------------------|----------------------|-----------------|----------------------------|
| Column Part No.: | 054427 | | |
| Phase: | BP20, 0.25 µm film | Detector: | FID |
| Column: | 30 m x 0.25 mm ID | Sensitivity: | 32 x 10 ⁻¹² AFS |
| Initial Temp: | Isothermal at 155 °C | Injection Mode: | Split |



GC Columns and Applications

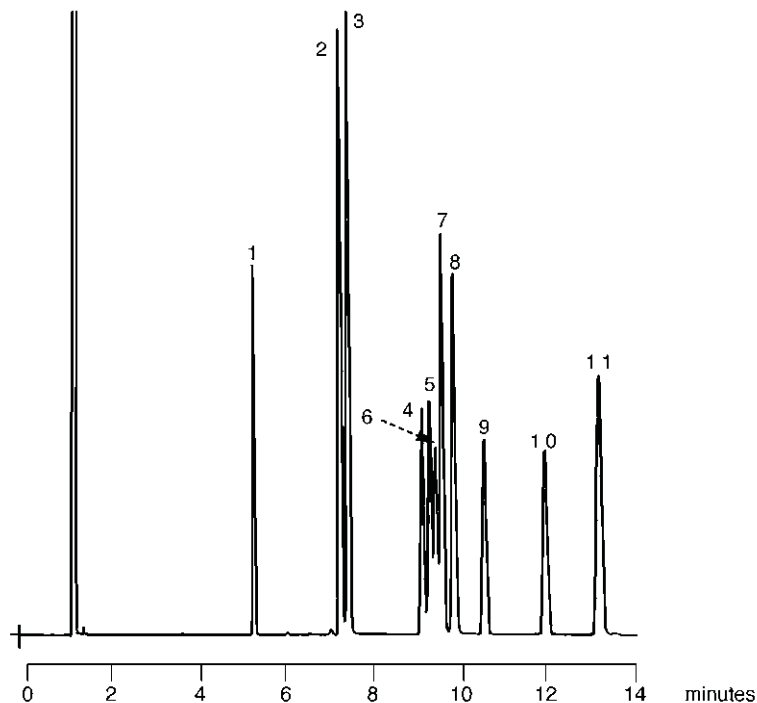

Components


1. 2,6-Xylenol
2. o-Cresol
3. Phenol
4. o-Ethylphenol
5. 2,5-Xylenol
6. p-Cresol
7. 2,4-Xylenol
8. m-Cresol
9. 2-iso Propylphenol
10. 2,3-Xylenol
11. 3,5-Xylenol + p-Ethylphenol

Notes: BP20 column completely resolves the three cresol isomers.

ACI 02 | Analysis of Organic Acids in Water on BP21

| | | | |
|-------------------------|-------------------|-----------------|----------------------------|
| Column Part No.: | 054477 | | |
| Phase: | BP21, 0.5 µm film | Final Temp: | 180 °C, 5 min |
| Column: | 30 m x 0.53 mm ID | Detector: | FID |
| Initial Temp: | 85 °C, 0 min | Sensitivity : | 64 x 10 ⁻¹² AFS |
| Rate: | 6 °C/min | Injection Mode: | On-Column |

Notes: On-column injection and the addition of a 0.03 M Oxalic acid (2%) to the injection solution increases the acidity of the column to allow lactic acid to be detected.

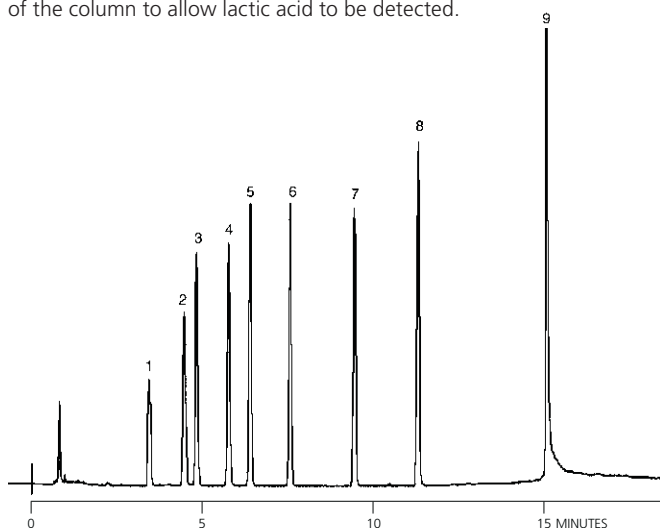


Components

1. Acetic Acid
2. Propanoic Acid
3. iso-Butyric Acid
4. n-Butyric Acid
5. iso-Valeric Acid
6. n-Valeric Acid
7. n-Caproic Acid
8. n-Heptanoic Acid
9. Lactic Acid






GC Columns and Applications

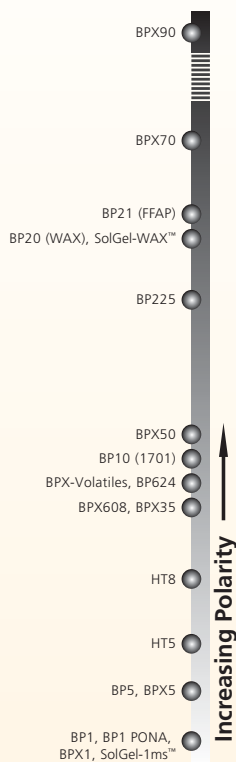

AMI 06 | Analysis of Aromatic Amines from Diazo Dyes on BPX35

| | |
|-------------------------|------------------------|
| Column Part No.: | 054701 |
| Phase: | BPX35 0.25 µm film |
| Azo Dyes standard: | 10 ppm solution in DCM |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp: | 50 °C, 2 min |
| Rate 1: | 15 °C to 240 °C |
| Rate 2: | 10 °C to 280 °C |
| Final Temp: | 280 °C, 25 min |
| Detector Type: | MS D |
| Carrier Gas: | He, 7.1 psi |
| Carrier Gas Flow: | 1.0 mL/min |

| | |
|--------------------------|----------------------------|
| Constant Flow: | On |
| Average Linear Velocity: | 36 cm/sec at 50 °C |
| Injection Mode: | Splitless |
| Purge on Time: | 1.0 min |
| Purge on (Split) | |
| Vent Flow: | 60 mL/min |
| Injection Volume: | 1 µL |
| Injection Temp: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part No.: | 092018 |

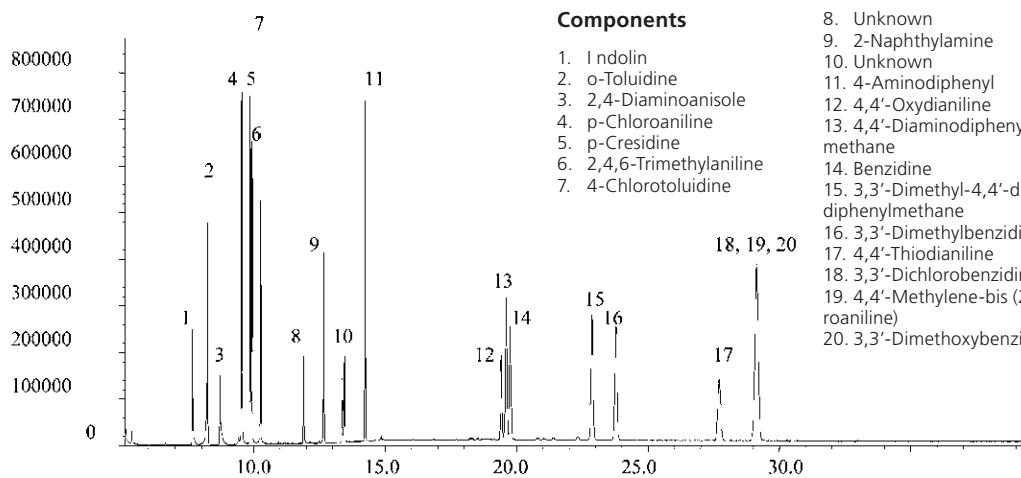


Components

- | | |
|---------------------------|---|
| 1. Indolin | 8. Unknown |
| 2. o-Toluidine | 9. 2-Naphthylamine |
| 3. 2,4-Diaminoanisole | 10. Unknown |
| 4. p-Chloroaniline | 11. 4-Aminodiphenyl |
| 5. p-Cresidine | 12. 4,4'-Oxydianiline |
| 6. 2,4,6-Trimethylaniline | 13. 4,4'-Diaminodiphenylmethane |
| 7. 4-Chlorotoluidine | 14. Benzidine |
| | 15. 3,3'-Dimethyl-4,4'-diaminodiphenylmethane |
| | 16. 3,3'-Dimethylbenzidine |
| | 17. 4,4'-Thiodianiline |
| | 18. 3,3'-Dichlorobenzidine |
| | 19. 4,4'-Methylene-bis(2-chloroaniline) |
| | 20. 3,3'-Dimethoxybenzidine |

AMI 03 | Analysis of Aromatic Amines on BP5

| | |
|-------------------------|-------------------|
| Column Part No.: | 054197 |
| Phase: | BP5, 1.0 µm film |
| Column: | 12 m x 0.53 mm ID |
| Initial Temp: | 60 °C, 0 min |
| Rate: | 10 °C/min |


| | |
|-----------------|-----------------|
| Final Temp: | 190 °C, 0 min |
| Detector: | FID |
| Sensitivity : | 128 x 10-12 AFS |
| Injection Mode: | Split |

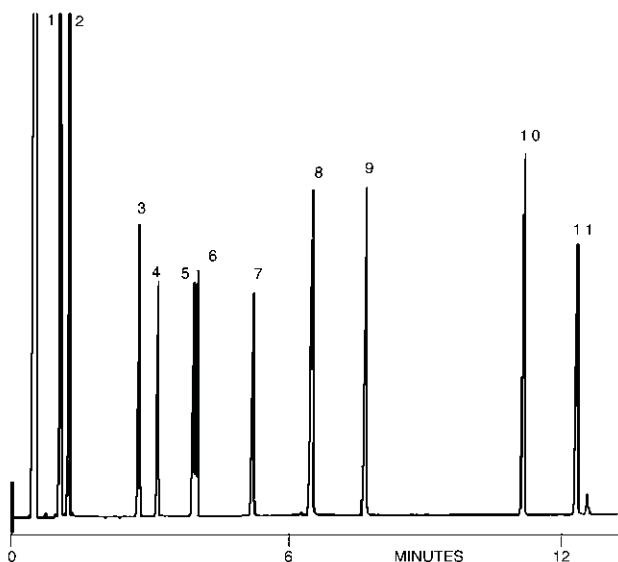

Components

1. Pyridine
2. 2-Methyl Pyridine
3. Aniline
4. Benzylamine
5. o-Toluidine
6. m-Toluidine
7. 2,6-Dimethylaniline
8. 1,4-Phenyldiamine
9. Nicotine
10. Biphenylamine
11. Bibenzylamine

AMI 04 | Analysis of Amines on BP1

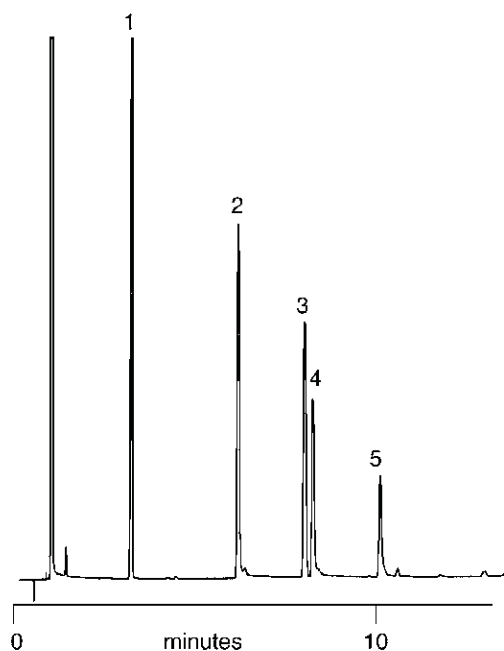

| | |
|-------------------------|-------------------|
| Column Part No.: | 054097 |
| Phase: | BP1, 3.0 µm film |
| Column: | 12 m x 0.53 mm ID |
| Initial Temp: | 70 °C |
| Rate: | 10 °C/min |
| Final Temp.: | 250 °C |
| Carrier Gas: | Nitrogen |
| Injection Volume: | 0.1 µL |

Components

1. Aniline
2. Decylamine
3. Dicyclohexylamine
4. Dodecylamine
5. Tetradecylamine




GC Columns and Applications

SOL 25 | Analysis of 22 Ketones on BPX35

| | | | |
|-------------------------|----------------------------|--------------------------|----------------------------|
| Column Part No.: | 054701 | Constant Flow: | On |
| Phase: | BPX35, 0.25 µm film | Average Linear Velocity: | 35 cm/sec at 40 °C |
| Sample: | 300 ppm in dichloromethane | Injection Mode: | Split |
| Column: | 30 m x 0.25 mm ID | Split Ratio: | 80:1 |
| Initial Temp: | 40 °C, 5 min. | Injection Volume: | 0.5 µL |
| Rate: | 10 °C/min to 170 °C | Injection Temp.: | 250 °C |
| Final Temp: | 170 °C, 5 min. | Liner Type: | 4 mm ID Single Taper Liner |
| Detector Type: | Mass Spectrometer | Liner Part Number: | 092017 |
| Carrier Gas: | He, 25.6 psi | Full Scan / SIM: | Full scan 45-450 |
| Carrier Gas Flow: | 1.6 mL/min. | | |


Components

- | | | |
|-------------------------|-------------------------|-------------------|
| 1. Acetone | 7. 3-Methyl-2-pentanone | 15. 3-Heptanone |
| 2. 2-Butanone | 8. 3-Hexanone | 16. 2-Heptanone |
| 3. 3-Methyl-2-butanone | 9. 2-Hexanone | 17. Cyclohexanone |
| 4. 2-Pentanone | 10. Mesityl oxide | 18. 2-Octanone |
| 5. 3-Pentanone | 11. 2-Methyl-3-hexanone | 19. 2-Nonanone |
| 6. 4-Methyl-2-pentanone | 12. Cyclopentanone | 20. 2-Decanone |
| | 13. 4-Methyl-2-hexanone | 21. 2-Undecanone |
| | 14. 5-Methyl-2-hexanone | 22. 2-Dodecanone |

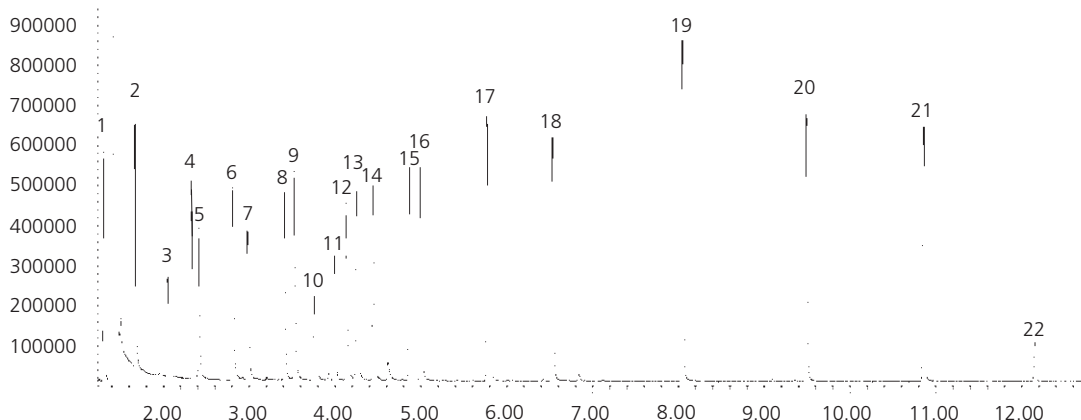



GC Columns and Applications

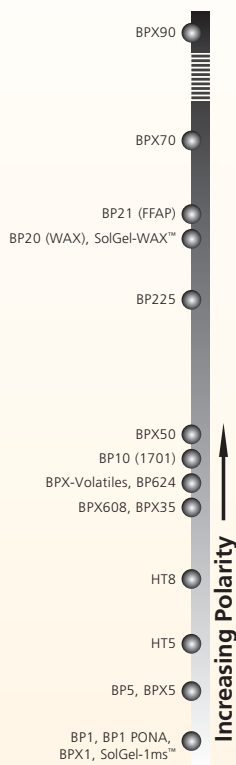


SOL 33 | Analysis of Ketones on Thick Film BPX5

| | |
|-------------------------|----------------------------|
| Column Part No.: | 054123 |
| Phase: | BPX5, 1.0 µm film |
| Sample: | 300 ppm in dichloromethane |
| Column: | 60 m x 0.25 mm ID |
| Initial Temp.: | 40 °C, 5 min. |
| Rate 1: 1 | 0 °C/min to 80 °C |
| Rate 2: | 30 °C/min to 260 °C |
| Final Temp: | 260 °C, 4 min. |
| Detector Type: | FID |
| Detector Temp.: | 360 °C |

| | |
|--------------------------|----------------------------|
| Carrier Gas: | He, 27.6 psi |
| Carrier Gas Flow: | 1.9 mL/min. |
| Constant Flow: | On |
| Average Linear Velocity: | 35 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 100:1 |
| Injection Volume: | 0.4 µL |
| Injection Tem.: | 250 °C |
| Liner Type: | 4 mm ID Single Taper Liner |
| Liner Part Number: | 092017 |

Components

- | | | |
|-------------------------|-------------------------|-------------------|
| 1. Ethanol | 8. 3-Methyl-2-pentanone | 17. 2-Heptanone |
| 2. Acetone | 9. 3-Hexanone | 18. Cyclohexanone |
| 3. 2-Butanone | 10. 2-Hexanone | 19. 2-Octanone |
| 4. 3-Methyl-2-butanone | 11. Mesityl oxide | 20. 2-Nonanone |
| 5. 2-Pentanone | 12. Cyclopentanone | 21. 2-Decanone |
| 6. 3-pentanone | 13. 2-Methyl-3-hexanone | 22. 2-Undecanone |
| 7. 4-Methyl-2-pentanone | 14. 4-Methyl-2-hexanone | 23. 2-Dodecanone |
| | 15. 5-Methyl-2-hexanone | |
| | 16. 3-Heptanone | |

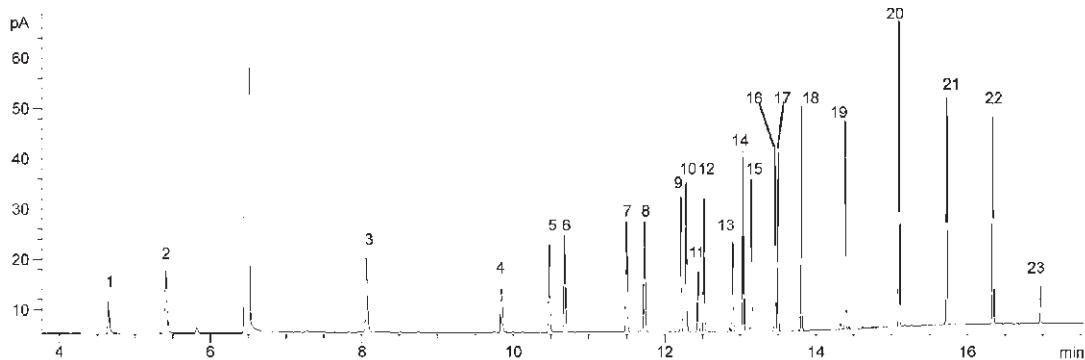


ALC 09 | Analysis of Phenols Mixture on BPX35




GC Columns and Applications

| | | | |
|------------------------|---------------------|---------------------------------|----------------------------|
| Column Part No: | 054701 | Constant Flow: | On |
| Phase: | BPX35, 0.25 µm film | Average Linear Velocity: | 35 cm/sec at 80 °C |
| Sample: | 200 ppm in methanol | Injection Mode: | Split |
| Column: | 30 m x 0.25 mm ID | Split Ratio: | 100:1 |
| Initial Temp: | 80 °C, 1 min | Injection Volume: | 1 µL |
| Rate 1: | 10 °C/min to 300 °C | Injection Temperature: | 250 °C |
| Final Temp: | 300 °C, 5 min | Liner Type: | 4 mm ID Single Taper Liner |
| Detector Type: | Mass Spectrometer | Liner Part No.: | 092017 |
| Carrier Gas: | He, 29.2 psi | Full Scan / SIM: | Full scan 45-450 |
| Carrier Gas Flow: | 1.7 mL/min. | | |

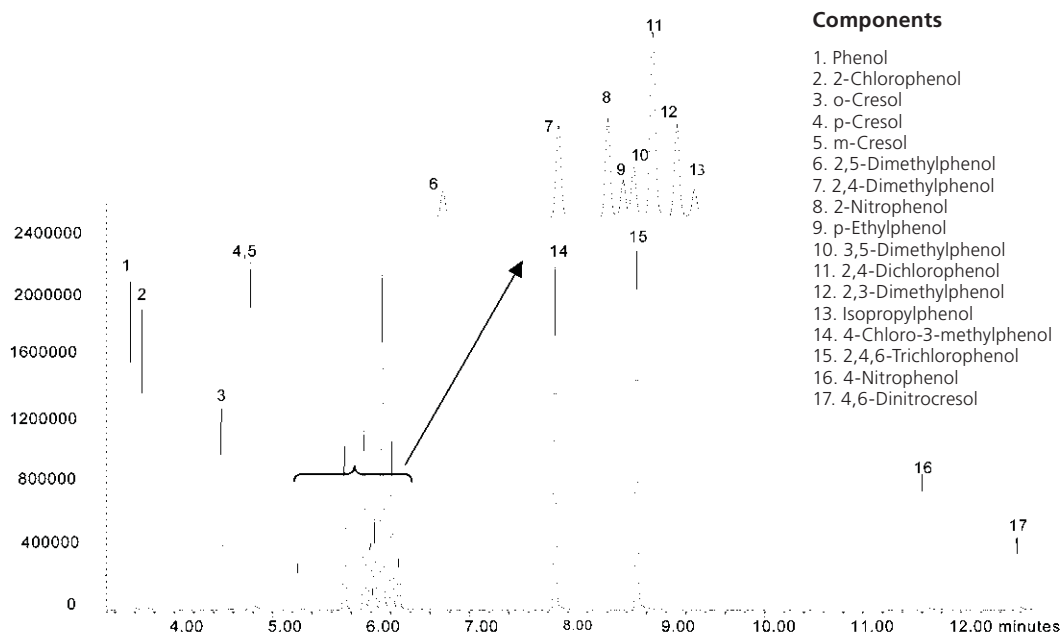



GC Columns and Applications

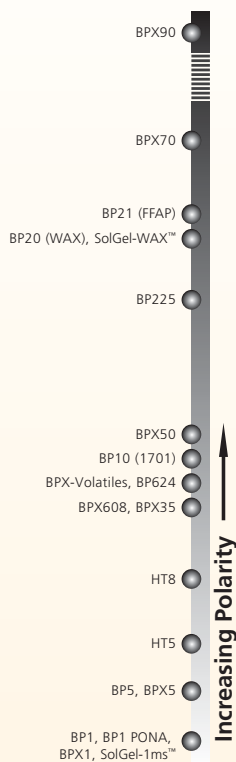


POL 06 | Analysis of Various Monomers on SolGel-WAX™

| | |
|-------------------------|--------------------------|
| Column Part No.: | 054796 |
| Phase: | SolGel-WAX, 0.25 µm film |
| Sample: | 250 ppm in Hexane |
| Column: | 30 m x 0.25 mm ID |
| Initial Temp: | 40 °C, 1 min. |
| Rate 1: | 10 °C/min to 250 °C |
| Final Temp: | 250 °C, |
| Detector Type: | FID |
| Detector Temp.: | 320 °C |
| Carrier Gas: | He, 16.6 psi |

| | |
|--------------------------|----------------------------|
| Carrier Gas Flow: | 1.6 mL/min. |
| Constant Flow: | On |
| Average Linear Velocity: | 35 cm/sec at 40 °C |
| Injection Mode: | Split |
| Split Ratio: | 80:1 |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Autosampler: | No |
| Liner Type: | 4 mm ID Single Taper Liner |
| Liner Part Number: | 092017 |

Components

- | | |
|--------------------------|---------------------------|
| 1. Ethyl acrylate | 6. Acrylic acid |
| 2. n-Butyl acrylate | 7. Hydroxypropyl acrylate |
| 3. n-Butyl methacrylate | 8. Methacrylic acid |
| 4. Styrene | 9. Unknown |
| 5. 2-Ethylhexyl acrylate | 10. Hydroxyethyl acrylate |
| | 11. Lauryl Methacrylate |

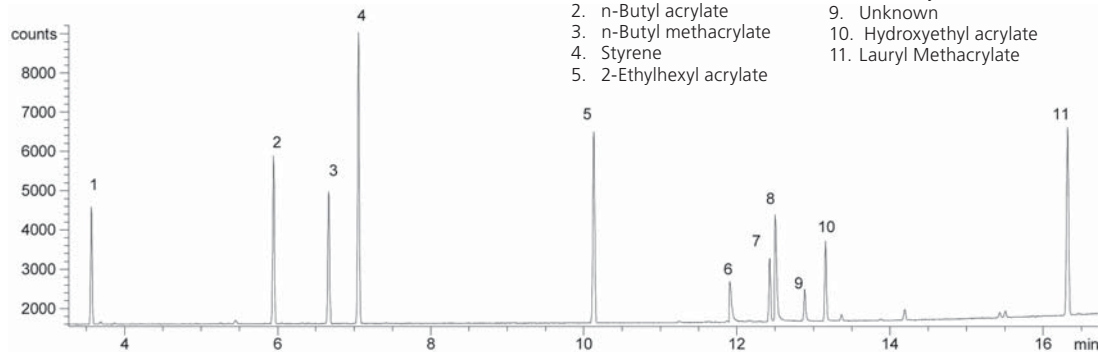

POL 01 | Analysis of Unreacted Monomers in Latex on BP20


| | |
|-------------------------|-------------------|
| Column Part No.: | 054488 |
| Phase: | BP20, 1.0 µm |
| Column: | 25 m x 0.53 mm ID |
| Initial Temp.: | 40 °C, 2 min |
| Rate: | 10 °C/min |

| | |
|-----------------|-----------------|
| Final Temp.: | 230 °C, 5 min |
| Injector Cond.: | Split, 280 °C |
| Detector: | FID, 280 °C |
| Carrier Gas: | Hydrogen, 4 psi |

Note: This was performed by heated headspace analysis.

Components

- Vinyl Acetate
- Ethyl Acrylate
- Monomethyl Methacrylate
- Butyl Acrylate
- Butyl Methacrylate
- Styrene
- Di-methylamino Ethyl-methacrylate
- 2-Ethyl Hexylacrylate
- Octanol
- Unknown
- 2-(acetoacetoxy) Ethyl Methacrylate
- Dibutyl Maleate
- Dicyclopentenloxyethyl Methacrylate

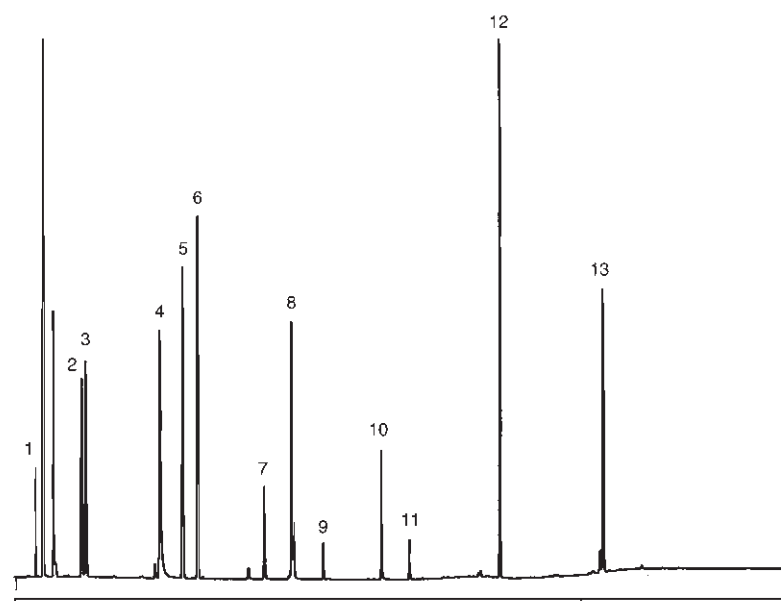



POL 05 | Pyrolysis of Styrene-isoprene Copolymer Pyrolysis of Polystyrene on BP1

| | |
|-------------------------|-----------------------|
| Column Part No.: | 054053 |
| Phase: | BP1, 1.0 µm |
| Column: | 25 m x 0.22 mm ID |
| Initial Temp.: | 40 °C, 1 min |
| Rate: | 10 °C/min |
| Final Temp.: | 140 °C |
| Detector: | FID |
| Pyrolysis Temp.: | 550 °C |
| Carrier Gas: | H ₂ 10 psi |

| | |
|-------------------------|------------------------|
| Column Part No.: | 054065 |
| Phase: | BP1, 0.5 µm |
| Column: | 25 m x 0.32 mm ID |
| Initial Temp.: | 40 °C, 1 min |
| Rate: | 10 °C/min |
| Final Temp.: | 130 °C |
| Detector: | FID |
| Pyrolysis Temp.: | 800 °C |
| Carrier Gas: | H ₂ , 5 psi |




GC Columns and Applications

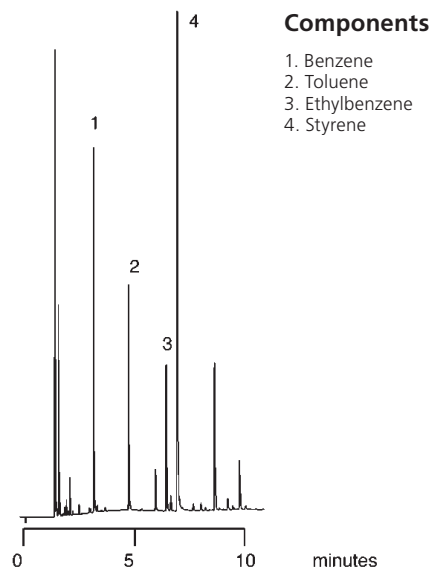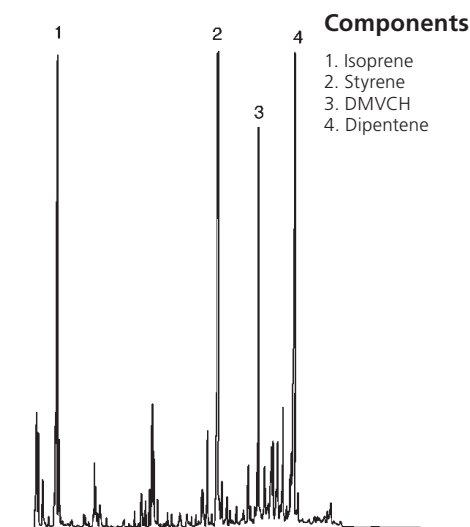

SOL 21 | Analysis of a Common Solvent Mixture on BP624


| | |
|-------------------------|--------------------------------|
| Column Part No.: | 054832 |
| Phase: | BP624, 1.8 µm film |
| Alcohol mix: | 1000 ppm in Dimethyl Sulfoxide |
| Column: | 30 m x 0.32 mm ID |
| Initial Temp: | 32 °C, 9 min. |
| Rate: | 30 °C/min to 190 °C |
| Final Temp: | 190 °C, 0 min. |
| Detector Type: | FID |
| Carrier Gas: | He, 9.6 psi |
| Carrier Gas Flow: | 2.2 mL/min. |

| | |
|--------------------------|----------------------------|
| Constant Flow: | On |
| Average Linear Velocity: | 34 cm/sec at 32 °C |
| Injection Mode: | Split |
| Split Ratio: | 100:1 |
| Injection Volume: | 0.2 µL |
| Injection Temperature: | 250 °C |
| Autosampler: | No |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

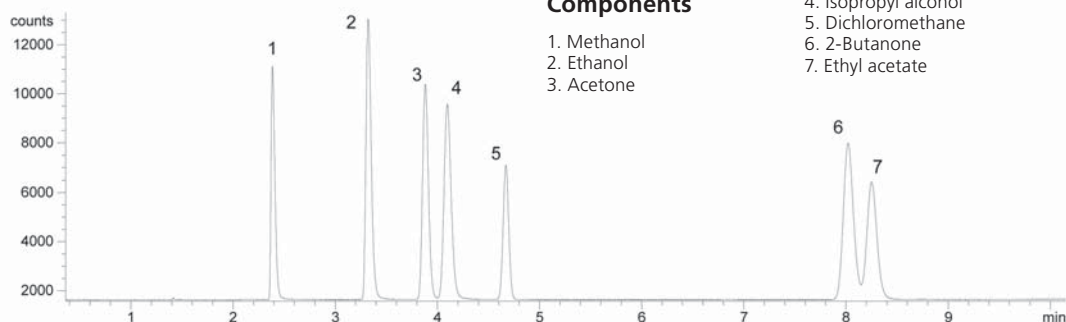




GC Columns and Applications

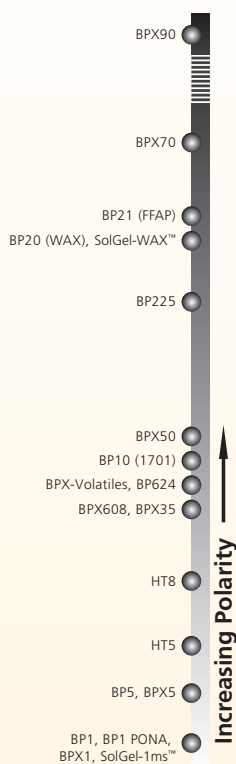

ENV 52 | Industrial Solvents on SolGel-WAX™

| | | | |
|--------------------------|--|----------------------------|--------------------|
| Column Part No. | 054797 | Constant Flow: | On |
| Phase: | SolGel-WAX™, 0.5 µm film 30 m x 0.32 mm ID | Pressure: | 8.4 psi |
| Split / Splitless | | Column Flow: | 1.84 mL/min |
| Injector Temp: | 240 °C | Linear Velocity: | 30 cm/sec at 35 °C |
| Injection Volume: | 0.1 µL | Initial Temp.: | 35 °C |
| Autosampler Syringe: | 0.5 µL Removable Needle Part No. 000410 | Initial Time: | 3 min |
| Septa: | Auto-Sep T™ Part No. 041882 | Rate 1: | 15 °C/min |
| Injection Type: | Split | Final Temp. 1: | 230 °C |
| Purge On Time: | NA | Hold Time: | 4 min |
| Purge On (Spilt) Vent: | 150 mL/min | Run Time: | 20.00 min |
| Split Ratio: | 83 to 1 | Detector Parameters | |
| Liner Type: | Single taper Part No. 092017 | Detector Type: | FID at 270 °C |
| Carrier Gas: | He | | |

Sample Description: Industrial solvents mix, 25 to 50 ng per component on column

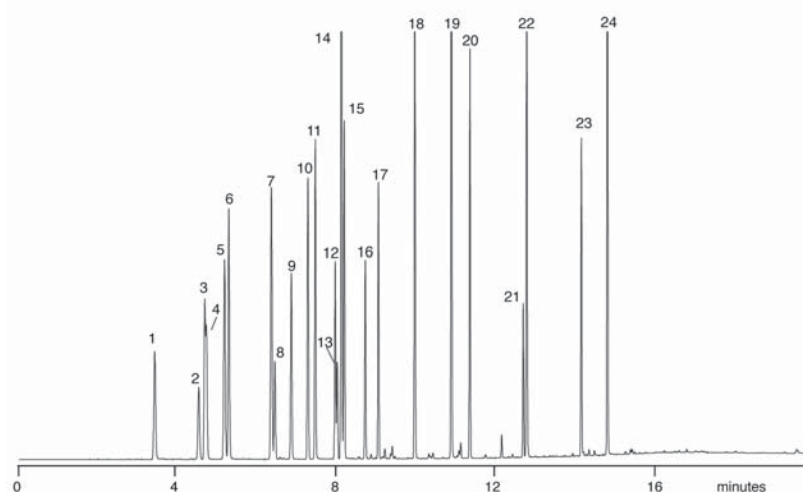


Components

1. Acetone
2. Ethyl acetate
3. Methyl ethyl ketone
4. Contaminant
5. iso-Propanol
6. Ethanol
7. Methyl isobutyl ketone
8. Toluene
9. Butyl acetate
10. iso-butanol
11. Propylene glycol monomethyl ether
12. n-Butanol
13. Ethyl benzene
14. p-Xylene
15. m-Xylene
16. o-Xylene
17. Butyl Cellosolve acetate
18. Cyclohexanone
19. Butyl Cellosolve
20. Butyl glycol acetate
21. Hexyl Cellosolve
22. Isophorone
23. Butyl Carbitol
24. Benzyl alcohol

SOL 04 | Acrylic Acid/Acrylamide Analysis on BP21

| | |
|-------------------------|-------------------|
| Column Part No.: | 054473 |
| Phase: | BP21, 0.5 µm film |
| Column: | 12 m x 0.53 mm ID |
| Initial Temp: | 75 °C, 0.5 min |
| Rate: | 10 °C/min |
| Final Temp: | 150 °C |
| Detector: | FID, 280 °C |
| Injection Mode: | On-Column |
| Carrier Gas: | He, 6 psi |


Notes: When response of acrylic acid is low, removal of 30 cm from the front of the column will correct this loss. On-column injection is recommended or polymerization of acrylic acid may occur.

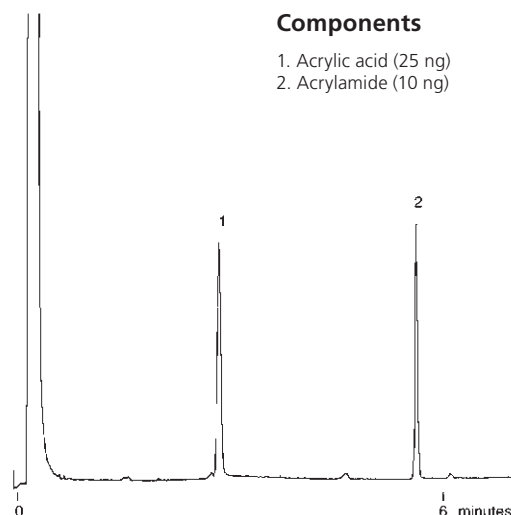

Components


1. Acrylic acid (25 ng)
2. Acrylamide (10 ng)

TP-0138-C | Analysis Of Polybrominated Diphenyl Ethers on BP1

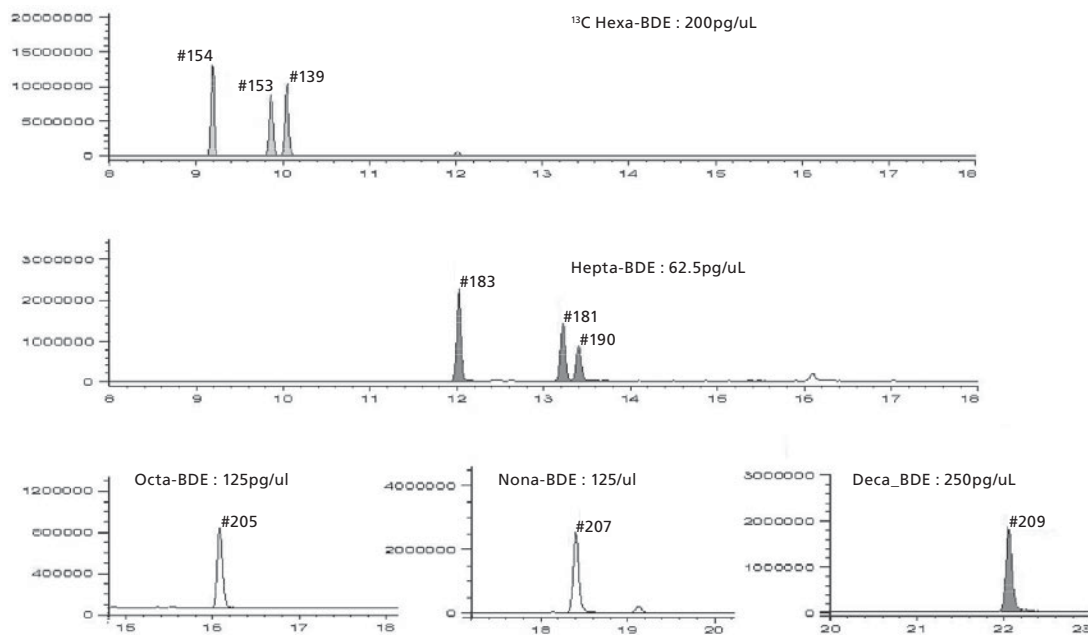

SGE would like to thank the Japan Food Research Centre for evaluating the BP1 column, SGE Japan and Chemicals Evaluation and Research Institute, Japan Toshiyuki KATAOKA, Masahiro AKIBA and Shinnichi KUDO.

TP-0138-C | Analysis Of Polybrominated Diphenyl Ethers on BPX5

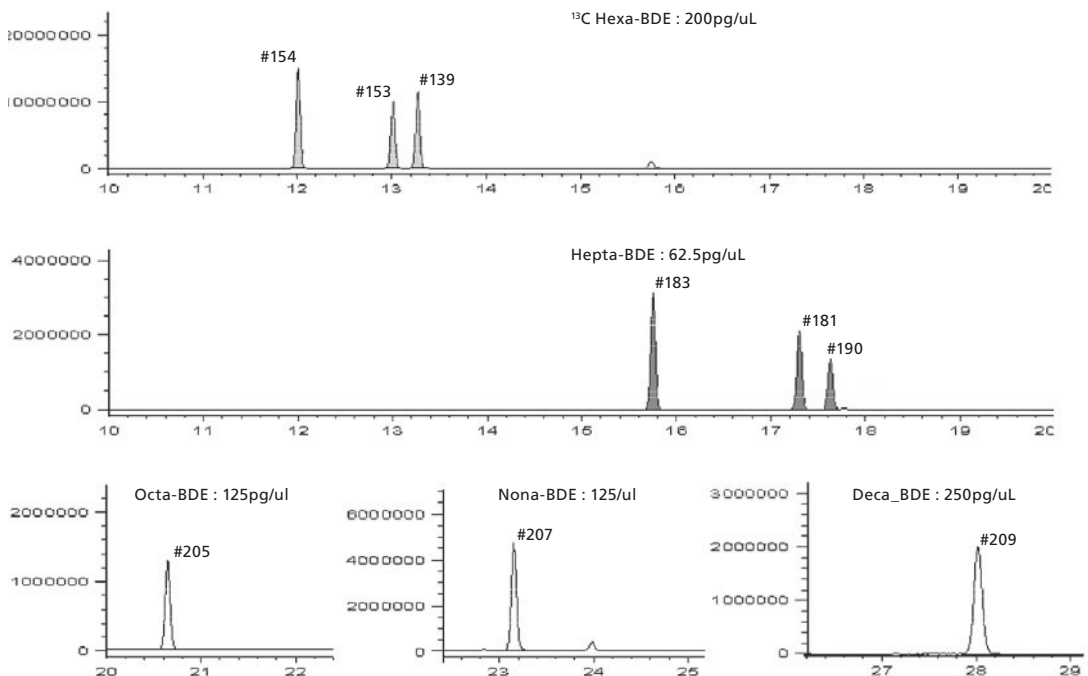

SGE would like to thank SGE Japan and Chemicals Evaluation and Research Institute, Japan Toshiyuki KATAOKA, Masahiro AKIBA and Shinnichi KUDO.




GC Columns and Applications







GC Columns and Applications

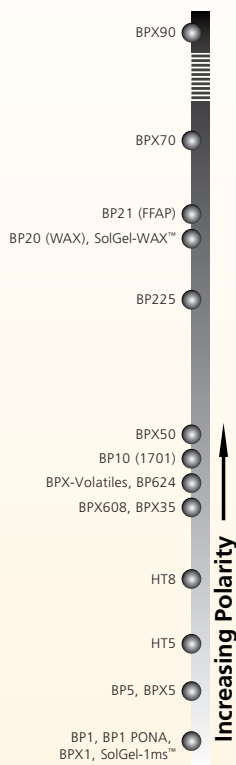

TP-0138-C | Analysis Of A Mixture Of Pentachlorobiphenyls on HT8-PCB

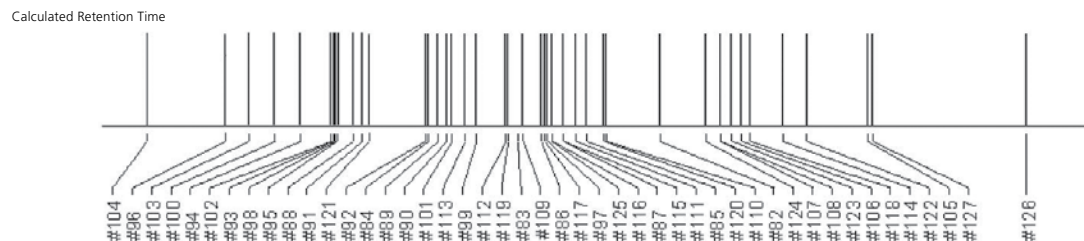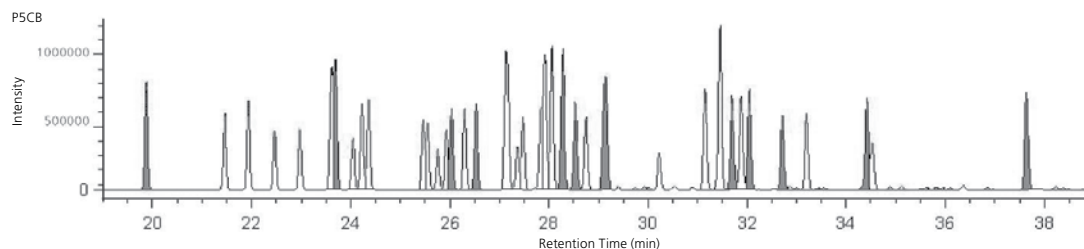

The separation of a mixture of pentachlorobiphenyls using an HT8-PCB column. Elution order calculated for the 5CBs from structure activity relationships based on coplanarity and confirmation, steric factors and electron density show a high correlation with experimental results.

SGE would like to thank T. Nakano, C. Matsumura and M. Tsurukawa at Hyogo Prefectural Institute of Public Health and Environmental Sciences, for providing the PCBs on HT8-PCB data.

TP-0138-C | Analysis Of A Mixture Of PBDD, PCDD And PBDF on BPX70


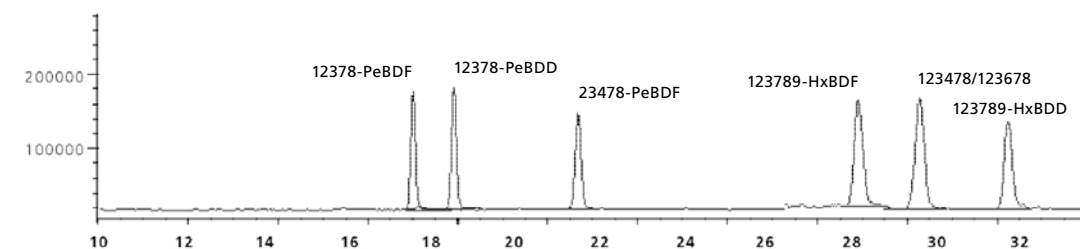


Figure 4. The separation of a mixture of PBDD and PBDF on a BPX70 column. The mixture was separated using the π - π interaction between the compounds and the cyano phase of the BPX70 column.


SGE would like to thank Toshiyuki Kataoka, Masahiro Akiba and Shinnichi Kudo of the Chemicals Evaluation and Research Institute, Japan, and SGE Japan, for providing the chromatograms of PBDEs on the ENV-5 and BPX70 columns.

PHA 14 | Analysis of Drugs of Abuse on BPX35

| | | | |
|-------------------------|---------------------|--------------|---------------|
| Column Part No.: | 054711 | Temp 2: | 200 °C |
| Phase: | BPX35, 0.25 µm film | Rate 2: | 7 °C/min |
| Column: | 25 m x 0.22 mm ID | Temp 3: | 295 °C |
| Initial Temp.: | 80 °C | Rate 3: | 20 °C/min |
| Rate 1: | 15 °C/min | Final Temp.: | 340 °C, 6 min |

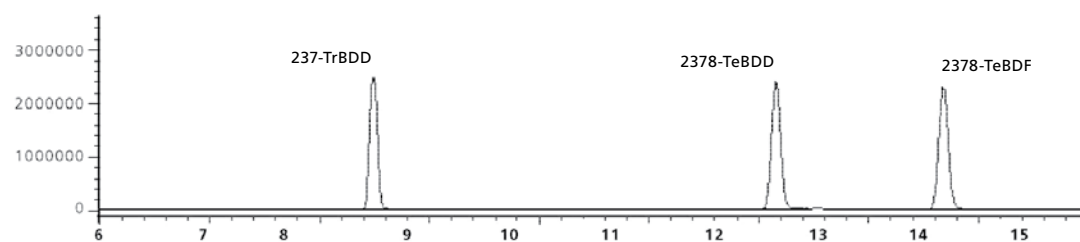

GC Columns and Applications

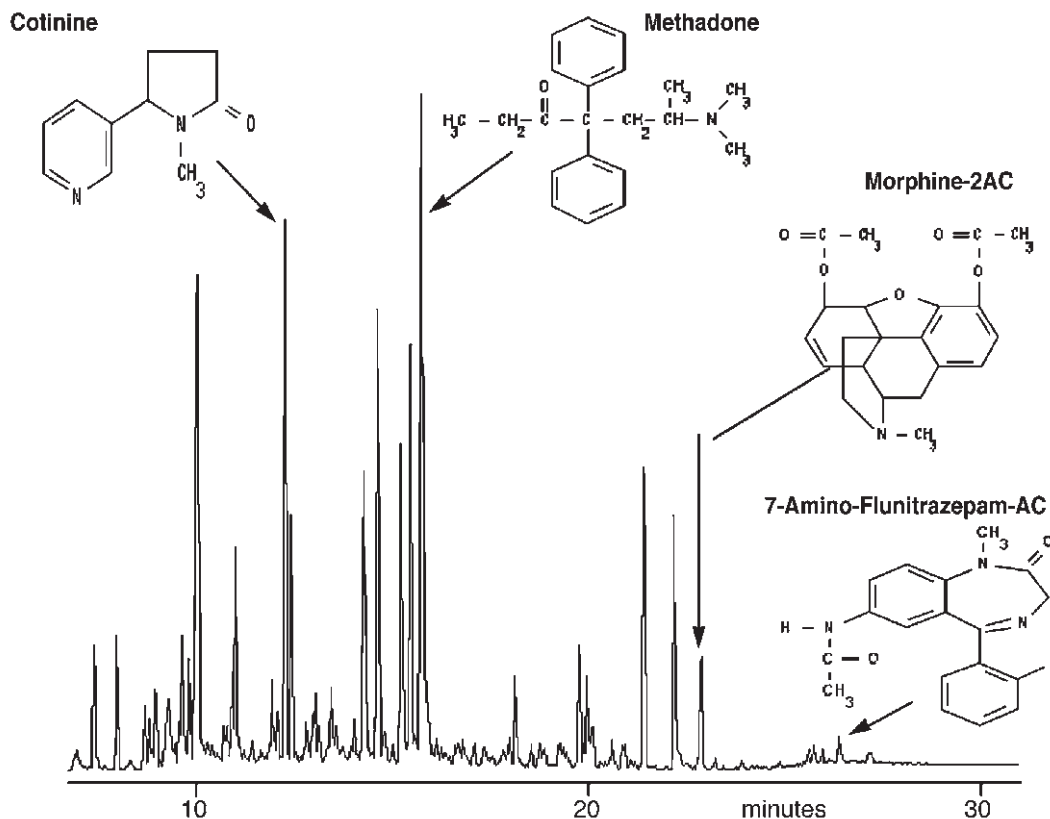


PHA 09 | Analysis of Tricyclic Antidepressants on BPX35

| | |
|-------------------------|-------------------|
| Column Part No.: | 054711 |
| Phase: | BPX35, 0.25 µm |
| Column: | 25 m x 0.22 mm ID |
| Initial Temp.: | 210 °C, 1 min |
| Rate: | 5 °C/min |
| Final Temp.: | 280 °C |
| Carrier Gas: | Helium, 150 kpa |
| Injection Mode: | Split (20:1) |
| Detector: | FID, 380 °C |

Components

1. Amitriptyline
2. Trimipramine
3. Nortriptyline
4. Doxepin
5. Desipramine

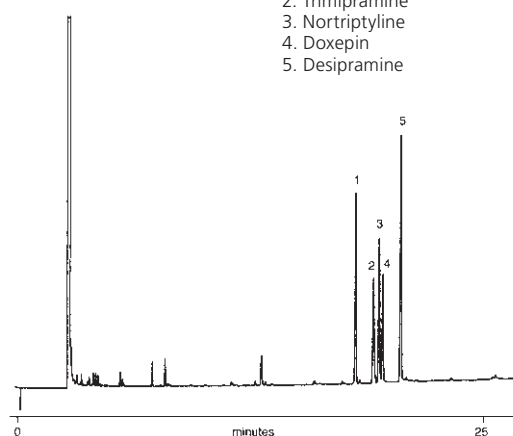


Note: BPX35 is a low bleed, chemically inert phase which allows trace analysis to occur.






GC Columns and Applications

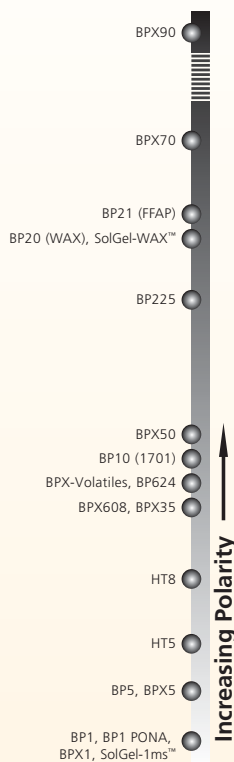

PHA 19 | Analysis of a Variety of Antidepressant and Anticonvulsant Drugs on BPX50

| | |
|-------------------------|----------------------|
| Column Part No.: | 054751 |
| Phase: | BPX50, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Sample: | 5-10 ppm in methanol |
| Initial Temp: | 150 °C, 0.5 min |
| Rate 1: | 10 °C/min to 180 °C |
| Rate 2: | 1.5 °C/min to 220 °C |
| Rate 2: | 30 °C/min to 260 °C |
| Final Temp: | 260 °C, 5 min |
| Detector Type: | FID |
| Detector Temp.: | 320 °C |
| Carrier Gas: | He, 25.7 psi |

| | |
|-----------------------------|----------------------------|
| Carrier Gas Flow: | 1.8 mL/min. |
| Constant Flow: | On |
| Average Linear Velocity: | 35 cm/sec at 40 °C |
| Injection Mode: | Splitless |
| Purge on Time: | 0.5 min |
| Purge on (Split) Vent Flow: | 60 mL/min |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Liner Type: | 4 mm ID Single Taper Liner |
| Liner Part Number: | 092017 |
| Full Scan / SIM: | Full scan 45-450 |

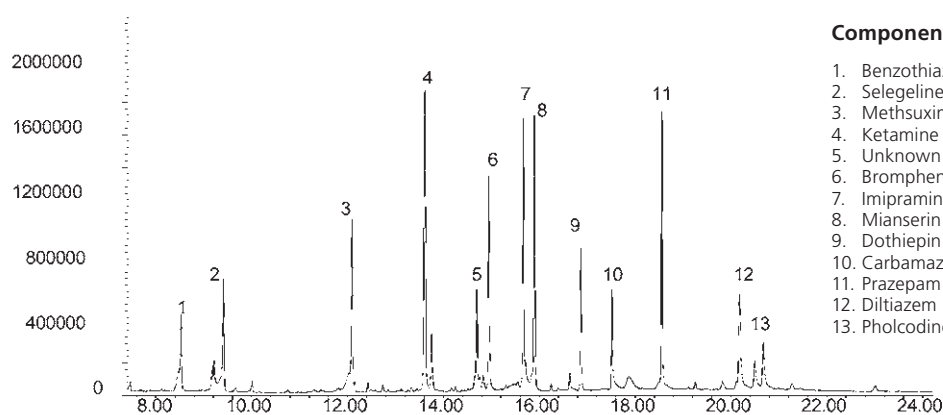

Components

1. Benzothiazole
2. Selegeline
3. Methsuximide
4. Ketamine
5. Unknown
6. Brompheniramine
7. Imipramine
8. Mianserin
9. Dothiepin
10. Carbamazepine
11. Prazepam
12. Diltiazem
13. Pholcodine


PHA 13 | Analysis of Blood Alcohol on BP20

| | |
|-------------------------|----------------------------|
| Column Part No.: | 054442 |
| Phase: | BP20, 1.0 µm film |
| Column: | 25 m x 0.32 mm ID |
| Initial Temp: | Isothermal, 60 °C |
| Detector: | FID |
| Sensitivity: | 64 x 10 ⁻¹² AFS |
| Injection Mode: | Split |

Note: The BP20 column allows the use of aqueous solutions.

Components


1. Acetone
2. Ethyl Acetate
3. Methanol
4. iso-Propanol
5. Ethanol
6. n-Propanol

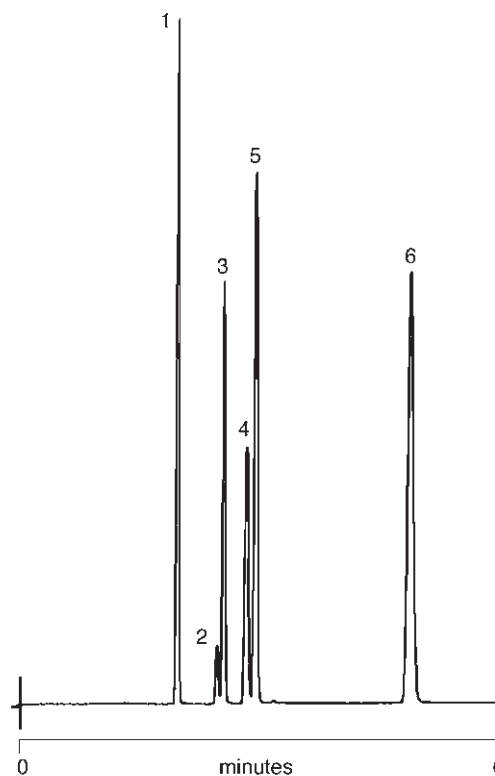

PHA 06 | Analysis of Basic Drug Screen on BPX5 (10-20 ng/component)

| | | | |
|-------------------------|---------------------|--------------|------------------------|
| Column Part No.: | 054131 | | |
| Phase: | BPX5, 1.0 µm | Final Temp.: | 310 °C |
| Column: | 25 m x 0.53 mm I.D. | Detector: | FID |
| Initial Temp.: | 120 °C | Injector: | Split, 240 °C |
| Rate: | 10 °C/min | Carrier Gas: | H ₂ , 2 psi |

Note: The low bleed nature of the BPX5 allows trace analysis to be performed.

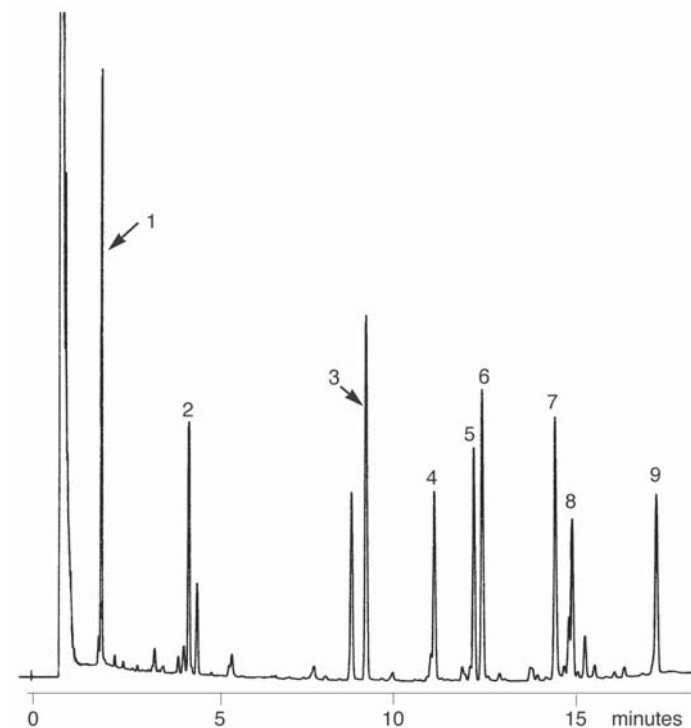


Components

1. Methamphetamine
2. Phendimetrazine
3. Phencyclidine
4. Mepivocaine
5. Methaqualone
6. Amitriptyline
7. Codeine
8. Diazepam
9. Fentanyl



GC Columns and Applications

PHA 08 | Underivatized Steroid Analysis on BPX5

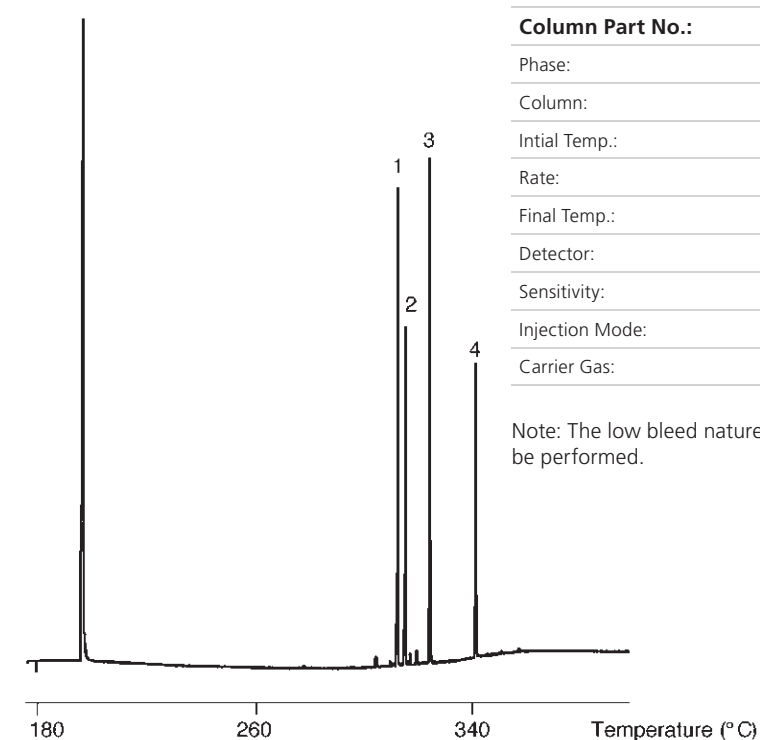

| | |
|-------------------------|----------------------------|
| Column Part No.: | 054113 |
| Phase: | BPX5, 0.25 µm |
| Column: | 25 m x 0.22 mm ID |
| Initial Temp.: | 180 °C |
| Rate: | 8 °C/min |
| Final Temp.: | 350 °C, 10 min |
| Detector: | FID |
| Sensitivity: | 32 x 10 ⁻¹² AFS |
| Injection Mode: | Split |
| Carrier Gas: | H ₂ , 10 psi |

Note: The low bleed nature of the BPX5 allows trace analysis to be performed.


Components

1. Testosterone
2. Pregnenolone
3. Progesterone
4. Cholesterol






GC Columns and Applications

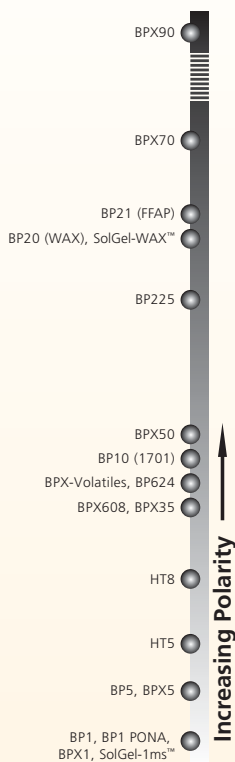

PHA 15 | Analysis of Horse Racing Test Mix on BPX5

| | |
|-------------------------|---------------------|
| Column Part No.: | 054101 |
| Phase: | BPX5, 0.25 µm film |
| Column: | 30 m x 0.25 mm ID |
| Horse Racing standard*: | 10 ppm in methanol |
| Initial Temp: | 75 °C, 2 min |
| Rate 1: | 15 °C/min to 300 °C |
| Rate 2: | 20 °C/min to 320 °C |
| Final Temp: | 320 °C, 8 min. |
| Detector Type: | Mass Spectrometer |
| Carrier Gas: | He, 14.5 psi |
| Carrier Gas Flow: | 1.5 mL/min |


| | |
|--------------------------|----------------------------|
| Constant Flow: | On |
| Average Linear Velocity: | 45 cm/sec at 75 °C |
| Injection Mode: | Splitless |
| Purge on Time: | 0.5 min |
| Purge on (Split) | |
| Vent Flow: | 60 mL/min |
| Injection Volume: | 1 µL |
| Injection Temperature: | 250 °C |
| Liner Type: | 4 mm ID Double Taper Liner |
| Liner Part Number: | 092018 |

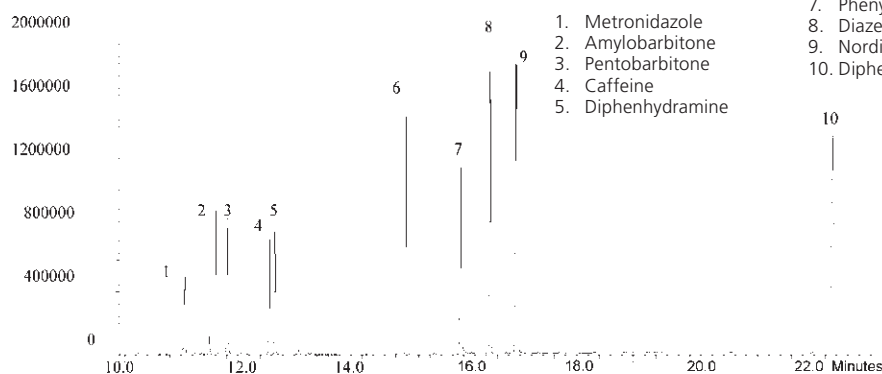

Components

- | | |
|--------------------|-------------------|
| 1. Metronidazole | 6. Trimipramine |
| 2. Amylobarbitone | 7. Phenytoin |
| 3. Pentobarbitone | 8. Diazepam |
| 4. Caffeine | 9. Nordiazepam |
| 5. Diphenhydramine | 10. Diphenoxylate |

PHA 03 | Analysis of Alkaloids on BP5

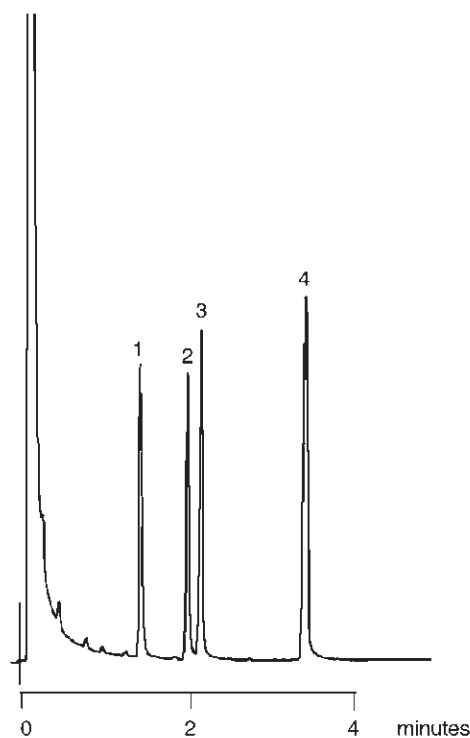

| | |
|-------------------------|-----------------------------|
| Column Part No.: | 054198 |
| Phase: | BP5, 1.0 µm film |
| Column: | 25 m x 0.53 mm ID |
| Initial Temp.: | 200 °C, 0 min |
| Rate: | 25 °C/min |
| Final Temp: | 300 °C, 0 min |
| Detector: | FID |
| Sensitivity: | 128 x 10 ⁻¹² AFS |
| Injection Mode: | Split |

Note: A 0.53 mm ID column can be used to screen samples rapidly.


Components

1. Cocaine
2. Codeine
3. Morphine
4. Quinine

PHA 10 | Underivatized Barbiturates on BP5



GC Columns and Applications

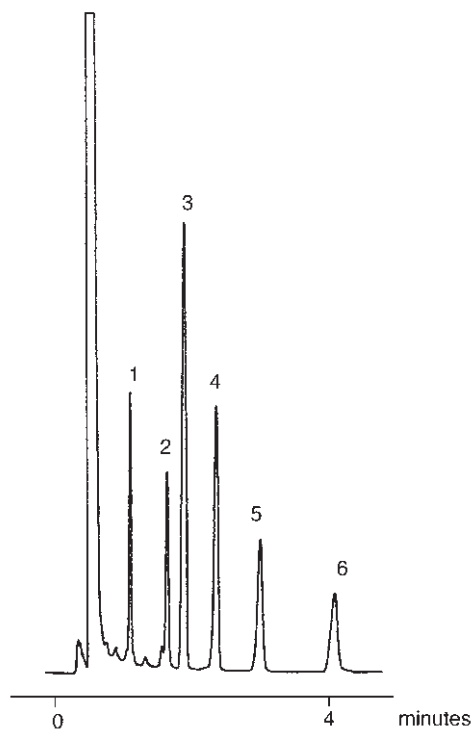


| | |
|-------------------------|---------------------|
| Column Part No.: | 054197 |
| Phase: | BP5, 1.0 µm |
| Column: | 12 m x 0.53 mm I.D. |
| Temp: | 195 °C |
| Carrier Gas: | Hydrogen |
| Carrier Flow: | 10 mL/min |
| Injection Volume: | 0.1 µL |

Note: A 0.53 mm ID column can be used to screen samples rapidly.

Components

1. Barbital
2. Butabarbital
3. Amobarbital
4. Pentabarbital
5. Secobarbital
6. Hexabarbital

PHA 04 | Analysis of Sedatives/Hypnotics on BP1

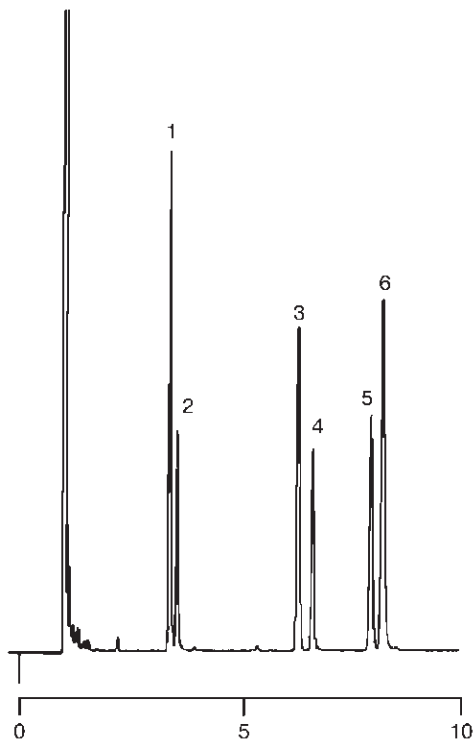

| | |
|-------------------------|------------------------------|
| Column Part No.: | 054087 |
| Phase: | BP1, 1.0 µm film |
| Column: | 25 m x 0.53 mm ID |
| Initial Temp.: | 180 °C, 0 min |
| Rate: | 10 °C/min |
| Final Temp.: | 250 °C, 3 min |
| Detector: | FID |
| Sensitivity: | 1024 x 10 ⁻¹² AFS |
| Injection Mode: | Split |

Components

1. Allobarbital
2. Aprobarbital
3. Diphenhydramine
4. Mephobarbital
5. Methapyrilene
6. Chlorpheniramine







GC Columns and Applications

PHA 01 | Analysis of Acid/Neutral Drugs on BPX35

| | | | |
|-------------------------|-------------------|-----------------|---------------|
| Column Part No.: | 054711 | | |
| Phase: | BPX35, 0.25 µm | Final Temp.: | 300 °C, 5 min |
| Column: | 25 m x 0.22 mm ID | Carrier Gas: | He, 150 kpa |
| Initial Temp.: | 100 °C, 1 min | Injection Mode: | Split, (20:1) |
| Rate: | 10 °C/min | Detector: | FID, 380 °C |

Note: BPX35 is a low bleed column with a maximum temperature of 360 °C. Very compatible with GC/MS systems.

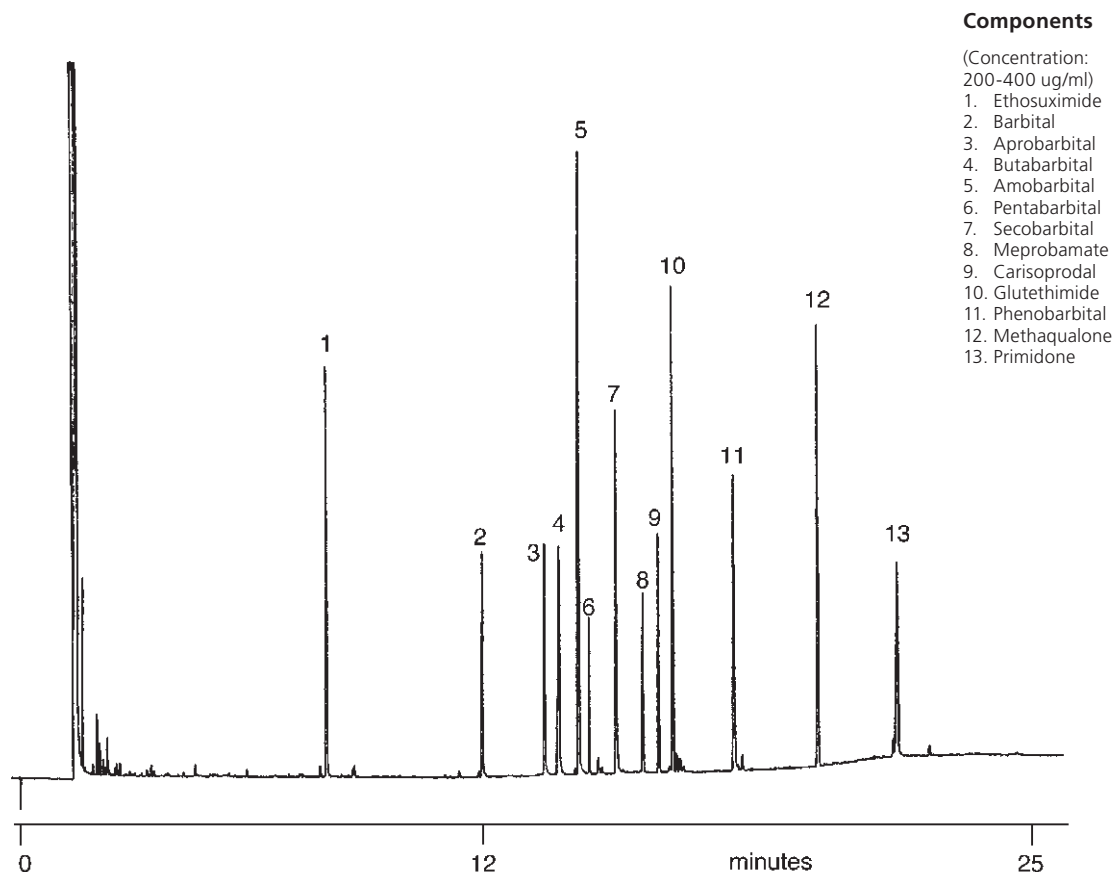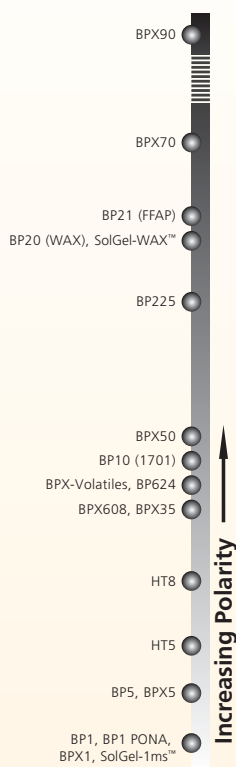

Components

- (Concentration: 200-400 ug/ml)
1. Ethosuximide
 2. Barbitol
 3. Aprobarbital
 4. Butabarbital
 5. Amobarbital
 6. Pentobarbital
 7. Secobarbital
 8. Meprobamate
 9. Carisoprodal
 10. Glutethimide
 11. Phenobarbital
 12. Methaqualone
 13. Primidone